

(12) PATENT  
(19) AUSTRALIAN PATENT OFFICE

(11) Application No. AU 200051953 B2  
(10) Patent No. 742417

(54) Title  
Analytical method and apparatus

(51)<sup>6</sup> International Patent Classification(s)  
G01N 021/55

(21) Application No: 200051953

(22) Application Date: 2000 .08 .11

(43) Publication Date : 2000 .11 .02

(43) Publication Journal Date : 2000 .11 .02

(44) Accepted Journal Date : 2002 .01 .03

(62) Divisional of:  
199858931

(71) Applicant(s)  
Biacore AB

(72) Inventor(s)  
Bengt Ivarsson

(74) Agent/Attorney  
DAVIES COLLISON CAVE, 1 Little Collins Street, MELBOURNE VIC 3000

(56) Related Art  
W0 90/05295

## ABSTRACT

An optical apparatus for examining thin layer structures on a surface for differences  
5 in respect of optical thickness, comprising:

a sensor unit having a sensor surface with a number of zones capable of exhibiting  
thin layer structures of varying optical thickness, particularly as the result of contact with a  
sample,

a light source for emitting a beam of light,

10 means for scanning the surface or area of a thin layer structure,

first photodetector means,

means for imaging light reflected from the different parts of the sensor surface onto  
the first photodetector means for detecting the intensities of the reflected light from the  
sensor surface,

15 means for sequentially or continuously scanning the light incident at the sensor  
surface over a range of incident angles and/or wavelengths,

means for determining each angle and/or wavelength of light impinging on the  
sensing surface,

evaluation means for determining from the relationship between detected intensity

20 of the reflected light and incident light angle and/or wavelength, the optical thickness of  
each zone of the sensor surface to thereby produce a morphometric image of the optical  
thickness of the sensor surface,

characterised in that the apparatus comprises second photodetector means, and that the  
means for determining the light angles and/or wavelengths comprise means for focusing a

25 part of monochromatic light reflected at the sensing surface onto the second photodetector  
means, wherein each position of the focused light on the second photodetector means is  
related to a specific angle and/or wavelength of the light incident at the sensing surface.

**AUSTRALIA**

**PATENTS ACT 1990**

**DIVISIONAL APPLICATION**

**NAME OF APPLICANT(S):**

**BIACORE AB**

**ADDRESS FOR SERVICE:**

DAVIES COLLISON CAVE  
Patent Attorneys  
1 Little Collins Street  
Melbourne, 3000.

**INVENTION TITLE:**

**"Analytical Method and Apparatus"**

The following statement is a full description of this invention, including the best method of performing it known to us:

## ANALYTICAL METHOD AND APPARATUS

### TECHNICAL FIELD

The present invention relates to a method and an apparatus for optical surface analysis of a sample area on a sensor surface.

### 5 BACKGROUND OF THE INVENTION

The interest for surface sensitive measuring techniques has increased markedly recently as several optical techniques have been developed for identifying and quantifying molecular interactions, which techniques do not require labelling. The most used optical technique so far is based on surface plasmon resonance, hereinafter  
10 frequently referred to as SPR.

The phenomenon of surface plasmon resonance, or SPR, is well known. In brief, SPR is observed as a dip in intensity of light for a specific wavelength reflected at a specific angle (as measured by, *e.g.*, a photodetector) from the interface between an optically transparent material, *e.g.*, glass, and a thin metal film, usually silver or gold,  
15 and depends on among other factors the refractive index of the medium (*e.g.*, a sample solution) close to the metal surface. A change of the real part of the complex refractive index at the metal surface, such as by the adsorption or binding of material thereto, will cause a corresponding shift in the angle at which SPR occurs, the so-called SPR-angle. For a specific angle of incidence, the SPR is observed as a dip in intensity of light at a  
20 specific wavelength, a change in the real part of the refractive index causing a corresponding shift in the wavelength at which SPR occurs.

To couple the light to the interface such that SPR arises, three alternative arrangements may be used, viz. either a metallized diffraction grating (see H. Raether in "Surface Polaritons", Eds. Agranovich and Mills, North Holland Publ. Comp.,  
25 Amsterdam, 1982), a metallized glass prism (Kretschmann configuration) or a prism in close contact with a metallized surface on a glass substrate (Otto configuration). In a SPR-based assay, for example, a ligand is bound to the metal surface, and the

---

interaction of this sensing surface with an analyte in a solution in contact with the surface is monitored.

Originally, collimated light was used for measuring the SPR-angle, the sensing area being restricted to the intersection of the collimated light beam and the metal surface. The apparatus used was based on mechanical goniometry with two movable mechanical axes carrying the illumination and detecting components, the rotational center of which was placed in the center of the sensor area, *i.e.*, one axis for the incident light and another axis for the reflected light which was detected by a single photodetector. A plane-sided coupling prism at total internal reflection condition was used to preserve the collimated beam inside the prism, which, however, introduced a refraction at non-orthogonal incidence at the prism, thereby introducing a beam-walk at the metal surface. A half-cylindrical coupling lens with orthogonal incidence of the optical axis of the light gave a fixed sensor area, however, introduced a beam-convergency, *i.e.*, a non-collimated or quasi-collimated beam inside the prism.

In a development, the movable opto-mechanical axis on the illumination side was eliminated by using a focused incident beam, so-called focused attenuated total reflection (focused ATR), as described by Kretschmann, Optics Comm. 26 (1978) 41-44, the whole angular range simultaneously illuminating a focal line or point of a given sensing surface. The use of a detector matrix for detecting the reflected light eliminated the movable opto-mechanical axis also on the reflectance side, providing a faster SPR-detection than that of the prior art. Such systems are described in, *e.g.*, EP-A-305 109 and WO 90/05295. In the latter, light beams reflected from a specific sub-zone at the sensor area are imaged anamorphically so that beams in one plane (the sagittal plane) create a real image on a specific detector-pixel row of a matrix detector, permitting the occurrence of a local surface binding reaction to be identified, while quantification of the reaction is obtained via angular data for a reflectance curve measured along the same pixel row, where the reflectance curve is created by beams in a plane (the meridian plane) normal to the first-mentioned plane. Thus, one dimension of the matrix detector is used for real imaging simultaneously as the other dimension is

used for only angular measurement. This permits only sub-zones arranged in a row to be simultaneously monitored and imaged.

In a variation of goniometry, the bulky mechanical axes were replaced by rotating or vibrating mirrors, respectively. A disadvantage of that approach is, however, that when scanning the incident angle by means of plane mirror, the point where the light beam hits the sensor surface will move along the internal reflection surface of the prism. This problem was avoided by using a combination of rotating mirror and focused SPR, e.g., as described by Oda, K., Optics Comm. 59 (1986) 361. In this construction, a first collimated beam of about 1 mm diameter impinges on the rotational center of a rotating mirror placed at the focal length of a focusing lens, thus producing a second quasi-collimated beam, the distance of which to the optical axis depends on the reflecting angle of the mirror. The second collimated beam is focused by a second focusing lens onto a prism base at total internal reflection conditions. During the rotation of the mirror, the angle of incidence at the approximately fixed sensor area is scanned for the quasi-collimated beam.

Another approach to obtain a fixed and also enlarged sample spot is proposed by Lenferink et al., "An improved optical method for surface plasmon resonance experiments", Sensors and Actuators B vol. 3 (1991) 261-265. This technique uses the combination of a collimated light beam illuminating a plane rotating mirror, a focusing cylindrical (convex) lens after the mirror and a half-cylinder lens for coupling the light to the sensing surface. By making the cylindrical lens focus the light on the focal surface of the coupling half-cylinder, using a relatively complex lens system, a collimated beam is obtained inside the coupling prism.

Other optical techniques similar to SPR are Brewster angle reflectometry (BAR) and critical angle reflectometry (CAR).

When light is incident at the boundary between two different transparent dielectric media, from the higher to the lower refractive index medium, the internal reflectance varies with angle of incidence for both the s- and p-polarized components. The reflected s-polarized component increases with the angle of incidence, and the p-polarized component shows a minimum reflectance at a specific angle, the Brewster



angle. The angle at which both s- and p-polarized light is totally internally reflected is defined as the critical angle. For all angles of incidence greater than the critical angle, total internal reflection (TIR) occurs.

Schaaf et al., Langmuir, vol. 3 (1987) describes Brewster angle reflectometry using a micro-controlled rotation table and a movable detector in scanning angle reflectometry around the internal Brewster angle to study a protein (fibrinogen) at a silica/solution interface. The use of movable optomechanical axes and a rotation table gives a slow measuring procedure, and the sensor area is restricted to the cross-section of the collimated light beam with the sensor surface being limited by the need for non-beam-walking.

A focusing critical angle refractometer, based on a wedge of incident light which strikes the line of measurement, including the critical angular interval to be measured, and which measures the one-dimensional refractive index profile along a focused line immediately adjacent to the glass wall of a liquid container is described by Beach, K. W., et al., "A one-dimensional focusing critical angle refractometer for mass transfer studies" Rev. Sci. Instrum., vol. 43, 1972. This technique is limited in that it enables only a one-dimensional sensor area, which is restricted to the cross-section of the light line with the sensor area.

In all the above described prior art methods for reflectometric measurements, the reflectometric signal obtained represents an average value for the sensor surface and the size of the sensor surface is restricted, or minimized, to the extension of the collimated or quasi-collimated narrow beam, or focusing point or line. Therefore, such SPR-based methods used to measure, for example, inter alia protein interactions are limited to quantitative information for sensing areas localized in one spot or one row of spots on the surface where a specific interaction takes place. Approaches to monitor a two-dimensional interaction pattern have been made for both macroscopic and microscopic SPR-based imaging of a sensing surface.

Thus, EP-A-341 928 discloses a method for monitoring a large SPR sensor area in real-time by scanning a small focused beam, of, e.g., 10  $\mu\text{m}$ , as a measuring sensing surface successively over the large area, more specifically a DNA

sequencing gel, for example  $20 \times 20 \text{ cm}^2$ , thereby making it possible to build up an image or picture of the sample distribution within the sequencing gel by means of a photodetector array. This method requires, however, the use of scanning mirrors for both addressing the sensor zones and scanning the angle and complex and expensive processing of angular and positional data from the mirror-scanners and photodetectors, which limits the detection rate.

Yeatman and Ash, *Electronic Letters* 23 (1987) 1091-1092, and *SPIE* 897 (1988) 100-107 disclose microscopic real imaging of the sensing surface, so called surface plasmon microscopy, or SPM. This was achieved by the use of SPR in the Kretschmann configuration with a triangular prism for imaging dielectric patterns deposited on a silver film with a lateral resolution of about  $25 \mu\text{m}$ , utilizing a focused beam in the form of a line scanned along the sensor surface. Also described is the use of an expanded laser beam at the resonance angle to illuminate a larger area and make a photograph of such an image by a positive lens in front of the photodetector. The illuminating beam is collimated and the angle of incidence is adjusted by rotating the triangular prism. The method is proposed to be used for the examination of metal films, biological and other superimposed monolayers.

Image processing methods for such SPM using a collimated beam and a lens inserted into the reflected beam to create an image of the sample distribution at the prism base are discussed by Yeatman and Ash in "Computerized Surface Plasmon Microscopy", *SPIE*, Vol. 1028 (1988) 231.

Okamoto and Yamaguchi have described a SPR-microscope wherein the position of a collimated beam, *SPIE* vol. 1319 (1990) 472-473, or a focused beam, *Optics Communications* 93 (1992) 265-270, is scanned across the sample surface in a Kretschmann configuration, the assembled point-SPR data thereby creating an image. In the focused beam alternative, a linear photodiode array is used for detection of the SPR-angle, in accordance with the principle of focused ATR as described earlier by Kretschmann, *supra*.

Drawbacks with mechanically scanned SPR-sampling includes that a high lateral resolution and high speed for "real time monitoring" demands a complex





and expensive scanning mechanics (due to the bulkiness of the illumination and detection device).


EP-A-469377 describes an analytical system and method for the determination of an analyte in a liquid sample based on surface plasmon imaging.

5 Surface plasmon images as a function of the angle of incidence are monitored by a CCD-camera and analyzed by an image-software. Algorithms are used for comparing the measured SPR-angle for different areas of the sensor surface for the purpose of eliminating the contribution from a non-specific binding, and for calibration of the response curve.

10 Rothenhausler and Knoll, Nature, 332 (1988) 615-617, demonstrates surface plasmon microscopy on organic films (a multilayer cadmium arachidate), based on SPR in a Kretschmann configuration. A simple lens is used to form an image of the sample/metal interface. A collimated beam (plane waves) illumination and a movable bulky optomechanical axis are used to change the angle of incidence.

15 In the above prior art arrangements for SPM, the angle of incidence is varied by the use of goniometry, either in a form where one or both optomechanical axes are moved (scanned) in relation to a fixed prism, or in a form using a movable optomechanical axis in combination with a rotating prism, the common rotation point being in the center of the prism sensor surface, and the angle of incidence being derived  
20 from the change in position or rotation of the mechanical axis through mechanical, electronic, electromagnetic or optical means. It is readily understood that such variation of the incident angle based on rotation of the mechanical axis carrying illuminating, imaging and detector modules is rather slow and inaccurate if not a complex and expensive design is provided.

25 Another approach is disclosed by Kooyman and Krull, Langmuir 7 (1991) 1506-1504, namely SPM using a small vibrating mirror in combination with a Kretschmann configuration to adjust the angle of incidence. A disadvantage is, however, that the probed spot is not stationary during the angular scan, i.e., all sites within a sensing area are not probed by light at an equal angle of incidence range, unless  
30 bulky optics is covering the sensing area at an excess.



Also microscopy based on Brewster angle measurements has been described. Hénon and Meunier, *Rev. Sci. Instrum.*, vol. 62 (1978) 936-939 discloses the use of a microscope at the Brewster angle for direct observation of first-order phase transitions in monolayers. In this case, external Brewster angle is measured, *i.e.*, no  
 5 internal reflection and no coupling prism, the camera plane being parallel with the sensor surface.

Similarly, Hönig and Mobius, *J. Phys. Chem.*, vol. 95 (1991) 4590-4592 describes the use of Brewster angle microscopy to study the air-water interface. Objects of about 3  $\mu\text{m}$  diameter could be visualized by video recording of p-polarized light  
 10 reflected under a fixed Brewster angle for the pure water surface.

A microscopic imaging ellipsometer has been described by Beaglehole, D., *Rev. Sci. Instrum.*, 59 (12) (1988) 2557-2559.

Multiple-angle evanescent wave ellipsometry, in the form of using rotating optical means and a rotating prism for the variation of incident angle, and a  
 15 phase-modulated ellipsometer, has been used for studying the polymer (polystyrene) concentration profile near a prism/liquid interface; see Kim, M.W., *Macromolecules*, 22, (1989) 2682-2685. Furthermore, total internal reflection ellipsometry in the form of stationary optical means at a single angle of incidence has been suggested for quantification of immunological reactions; see EP-A1-O 0 67 921 (1981), and EP-A1-O  
 20 278 577 (1988).

Azzam, R. M. A., *Surface Science* 56 (1976) 126-133, describes a use of evanescent wave ellipsometry, wherein both the intensity and polarization ellipse of the reflected beam can be monitored as functions of the angle of incidence, wavelength or time. Under steady state conditions, measurements as a function of wavelength and  
 25 angle of incidence can provide basic information on the molecular composition and organization of the (biological) cell periphery. In a dynamic time-varying situation, measurements as a function of time can resolve the kinetics of certain surface changes.

Abelès, F. et al., in *Polaritons*, Editor E. Burstein and F. De Martini, Pergamon Press, Inc., New York, 1974, 241-246, shows how extremely sensitive  
 30 surface plasmons are to very fine modifications of the surface, and the advantage of

then measuring not only the reflected amplitude, but also the ellipsometric parameters, amplitude and phase, of the reflected wave.

A focusing critical angle refractometer for measuring a one-dimensional refractive index profile being displayed in a graphic image for mass transfer studies has  
 5 been described by Beach, K.W., The Review of Scientific Instruments, 43, No. 6 (1972) 925-928. Since this apparatus uses one dimension in the image plane for a real image, and the other dimension for projecting the reflectance versus angle of incidence, it could not, however, provide a two-dimensional image of the refractive index distribution.

The prior art microscopy systems described above do not permit a  
 10 sufficiently rapid, sensitive and accurate scanning and measurement of the incident angle to permit highly quantitative multi-site real-time monitoring of a sensor surface. Further, they are only suitable for imaging a limited sensor area of up to about 1 x 1 mm<sup>2</sup>. They are also too laborative and operator-dependent to be used in a commercial analytical instrument.

15 More particularly, the prior art apparatuses and systems for SPR microscopy and Brewster angle microscopy use either a high inertia scanner in the form of a goniometer where one or both mechanical axes for the illumination side and the imaging side, respectively, are rotated in relation to a fixed prism, or a movable mechanical axis in combination with a rotating prism for scanning the optical axis, i.e.,  
 20 the angle of incidence. In case the illumination consists of a collimated beam of light, the incident angle is measured directly on the angle steering signal without using the incident light, e.g., on the control signal to the rotor-driving motor of a mirror, or by an electronic or optoelectronic angle sensor placed on or at the rotated axis. Alternatively, a galvanometric or resonant low inertia scanner is used to drive a vibrating mirror to  
 25 oscillate within a given calibrated angular range, determined by a given drive current, without monitoring the actual incident angle of the light.

The necessary high refractometric sensitivity for determining the refractive index of the sensor surface with an apparatus constructed according to the above prior art in a long-term accurate commercial analytical instrument could therefore  
 30 only be achieved with a very complex and expensive design.


The reference to any prior art in this specification is not, and should not be taken as, an acknowledgment or any form of suggestion that that prior art forms part of the common general knowledge in Australia.

## 5 SUMMARY OF THE INVENTION

It is an object of the present invention to overcome one or more of the above disadvantages and provide an optical method and apparatus that permits microscopic as well as large area analysis of the sensing surface of a sensor chip or plate with a high refractometric sensitivity and accuracy at high spatial resolution, or to at least provide a useful alternative to known methods and apparatus.



The above object may be provided by a large area or microscopy analytical apparatus of the above described types, as well as in others, by using part of the angular or wavelength-scanned light that illuminates the sensor chip for monitoring and determining the momentary incident angle or wavelength of the light.



As will be further explained below, this enables an improved quantitative measuring precision, accuracy and speed in the determination of the angle of incidence (alternatively wavelength) corresponding to the local reflection curve parameters, e.g., reflectance minimum, at the surface structures on the sensor surface, such as surface-distributed reaction sites.

The present invention provides an optical apparatus for examining thin layer structures on a surface for differences in respect of optical thickness, comprising:

- a sensor unit having a sensor surface with a number of zones capable of exhibiting thin layer structures of varying optical thickness, particularly as the result of contact with a sample,
- a light source for emitting a beam of light,
- optical means for coupling said light beam to said sensor unit,
- first photodetector means,
- means for imaging light reflected from said different parts of the sensor surface onto said first photodetector means for detecting the intensities of the reflected light from the sensor surface,



- 10 -

means for sequentially or continuously scanning said light incident at said sensor surface over a range of incident angles and/or wavelengths,

means for determining each angle and/or wavelength of light impinging on said sensing surface,

5 evaluation means for determining from the relationship between detected intensity of the reflected light and incident light angle and/or wavelength, the optical thickness of each zone of said sensor surface to thereby produce a morphometric image of the optical thickness of the sensor surface,

10 characterised in that the apparatus comprises second photodetector means, and that said means for determining said light angles and/or wavelengths comprise means for focusing a part of monochromatic light reflected at the sensing surface onto the second photodetector means, wherein each position of said focused light on said second photodetector means is related to a specific angle and/or wavelength of the light incident at the sensing surface.

15 The present invention also provides a method of using an optical apparatus as described above for examining thin layer structures on a surface for differences in respect of optical thickness, which method comprises:

irradiating the surface with light so that the light is internally or externally reflected at the surface,

20 imaging the reflected light on a first two-dimensional detector, sequentially or continuously scanning the incident angle and/or wavelength of the light over an angular and/or wavelength range,

measuring the intensities of light reflected from different parts of the surface and impinging on different on different parts of the detector, at at least a number of  
25 incident angles and/or wavelengths, the intensity of light reflected from each part of the surface for each angle and/or wavelength depending on the optical thickness of the thin layer structure thereon,



- 10A -

and determining from the detected light intensities at the different light incident angles and/or wavelengths an optical thickness image of the thin layer structures on the surface,

characterised in that part of the light reflected at said surface is detected on  
5 a second detector to determine the incident angle or wavelength of the polarised light irradiating the surface.

10  
15  
20  
25  
30



The term "optical thickness" as used herein defines a composite optical property of a material which is a function of both its physical thickness and its refractive index.

The term "surface structures" as used herein means any chemical, physical, 5 biophysical and/or biochemical structures of thin or other type on a sensor surface, especially structures produced via chemical or biochemical interactions with species immobilized on the sensor surface.

It is understood that in accordance with an embodiment of the present invention, a series of images of a sensor surface are created, one image for each specific 10 incident angle or wavelength. A part of the imaging detector, or a separate detector, is used for measuring the incident angle or wavelength. This will be described in more detail further below.

The light is usually polarized prior to hitting the photodetector. This may be accomplished by using a light source which emits polarized light or by placing a polarizer 15 between the light source and the detector.

In one basic embodiment of the invention, monochromatic angularly scanned light is used, and a main first part of the reflected collimated beam is used to produce a real image on a first main area of the matrix photodetector, while a second part of the reflected collimated beam is focused into a sharp line on a second specific minor linear area of the 20 matrix photodetector. During the angular scan of the collimated beam the change in angle of incidence is determined through the change in position of either the maximum, or the centroid of the focused light intensity detected by the detector elements along the linear detector area by use of an intensity-curve analysis algorithm.

In another basic embodiment of the invention, a scanned monochromatic light 25 at a fixed angle of incidence is used, and the second part of the reflected fixed colimated beam passes a wavelength dispersive element, and is then focused into a sharp point or line on a second specific minor linear area of said matrix detector.

---

During the wavelength scan of the beam the change in wavelength is determined through the change in position of either the maximum, or the centroid of the focused light intensity detected by the detector elements along the linear detector area by use of an intensity-curve analysis algorithm.

5 In a preferred embodiment, the present invention provides an improved reflectometric performance for an imaging method based on total internal reflection, such as *e.g.*, surface plasmon resonance (SPR), or external reflection, such as external Brewster angle spectroscopy or ellipsometry, by the use of a novel optical design which will be further described below and comprises a bifocal imaging system enabling  
10 simultaneous sensor zone resolution and projection of rays for measurement of the angle of incidence, and of the wavelength, on the same matrix photodetector array, and a low inertia mirror scanner system for a mainly stationary illuminated area of the sensor chip in combination with a total internal reflection element, or a grating, for coupling an evanescent wave to the sensor surface.

15 More particularly, such an apparatus may comprise an imaging system having two different focal lengths in the same plane of projection (meridian plane), together with an identical focal length for the sagittal plane and the dominating part of the meridian plane, and a common photodetector matrix array for image and angle monitoring. Preferably, the main part of the detector array lies in the real image plane  
20 of the imaging system, while a minor part of the detector matrix array lies in the back focal plane of the imaging system. Detector elements within the real image plane monitor light intensity originating from specific local spots at microscopic lateral resolution, while other detector elements within the back focal plane detect the position of the focused line, *i.e.*, the angle of incidence.

25 In an alternative form, the bifocal imaging enables detector elements within the real image plane to monitor light intensity originating from a specific local spot at microscopic lateral resolution, while other detector elements within the back focal plane detect the position of the focused line corresponding to the wavelength.

The reflected light intensity varies with the angle of incidence, mainly  
30 due to the angle dependent reflection coefficient, but may also vary due to a movement



of the illuminated area if the light intensity across the illuminating beam is not constant. By use of an approximately stationary illuminated sensor area, together with an image-intensity normalization algorithm, a highly resolved light intensity of the local reflectance curves may be detected, which enables a high resolution in the determined  
 5 angle/wavelength at the corresponding reflectance minima or maxima or centroid.

While it is preferred that the same detector array component is used for both image detection and angle or wavelength detection, separate detectors may, of course, also be used.

When both incident angle and wavelength of the light are to be  
 10 measured, the detector may be divided into two (smaller) parts, and a larger part, wherein one of the smaller parts is used for detection of the incident angle, and the other smaller part is used for detection of the wavelength, and the larger detector part is used for imaging.

Embodiments of the invention are characterized by an integral detection of both  
 15 image and incident light angle and/or wavelength to obtain a better accuracy and sensitivity in the multi-zone reflectometry and a faster analysis procedure than those obtained in the prior art. Thus, according to these embodiments, the same collimated light is used (i) to illuminate each point on the sensor surface with a practically identical angle of the incident light, permitting a minimum deviation (a maximum deviation of  $0.002^\circ$ ) within the whole sensor  
 20 area for a large angular/refractometric dynamic range, and (ii) to measure changes in this angle for each zone with a resolution of the order of  $0.0001^\circ$ .

Thus, by integrating into the structure (i) a detector for a highly resolved image of, for example, a multi-zone sensor surface, and (ii) a detector for the angle  
 25 and/or wavelength, respectively of the incident light, and thereby reduce the sources of error for the measurement of angle and wavelength, respectively, and their relation to a specific sensor subzone representation on the photodetector matrix, the following advantages may be obtained in relation to the prior art apparatus constructions:

- A higher resolution of absolute and relative reflectance minimum angle,
- 30 - a higher resolution of absolute and relative reflectance minimum wavelength,

- a higher image contrast and resolution of image contrast,
  - a higher frequency for reflectance image data detection,
  - a higher optomechanical robustness (less wear, lower maintenance cost),
  - a smaller total volume for the optomechanical apparatus, which permits an improved
- 5 (cheaper, quicker) thermostating, and thereby improved measuring system performance.

The apparatus according to the invention may use any of a number of optical principles for the scanning of the angle of incidence of the collimated beam, known to those skilled in art, including the principles described above in the description

10 of the prior art, as long as the beam deflecting principle selected provides an angularly scanned collimated beam incident on a sensor surface at total internal reflection conditions, in either a Kretschmann or Otto prism configuration, or a grating coupling configuration, during the probing of a mainly stationary area.

Exemplary such scanning principles are reflective beam steering through

15 mirrors or reflection diffraction gratings, and transmissive beam steering through refracting scanners, or through transmission diffraction gratings or transient gratings (acousto-optical scanning). These beam-steering principles may be combined into suitable scanner configurations known to a person skilled in the art.

Likewise, the optical system principle for the determination of reflection

20 versus angle and/or wavelength of incidence may be selected from a number of optical principles known to a person skilled in art, including those described above in the description of the prior art. Exemplary such optical principles are surface plasmon resonance (SPR), Brewster angle (both internal and external), ellipsometry angle (both internal and external), critical angle, and frustrated total reflection waveguide

25 resonance.

In the case of also an evanescent wave absorbing sample interaction with the sensing zone, the change in the complex refractive index corresponds not only to a shift in the SPR-angle or SPR-wavelength (related to the changed real part of the complex refractive index) but also to a shift in depth of the intensity at the resonance.

For sensor applications involving absorbance, the apparatus according to the invention may operate for reflectance-absorption imaging.

In the case of the incident light being coherent, a spatially heterogeneous sensing surface in terms of optical thickness or refractive index modulates the relative phase of the evanescent wave, creating a stationary interference pattern in the image or real image obtained. The incident light may after the total internal reflection interfere with light partially reflected at another interface of the sensor unit, *e.g.*, on the opposite side to the sensor surface substrate interface on the substrate. When, for example, a sample molecule is specifically bound to certain areas within this sensing surface, the interference fringes move into new positions. By tracking the position of specific fringes by use of image process software, in relation to the scanned angle or wavelength of incidence, the local surface concentration changes may be interferometrically monitored by the apparatus according to the invention. The interferometric feature of phase-sensitive evanescent wave detection may increase the refractometric sensitivity in, for example, interferometric surface plasmon resonance image analysis, or interferometric Brewster angle and critical angle image analysis.

Generally, the present invention creates an optically densitometrically (refractometrically) quantitated image of a sensing surface pattern in approximative real-time by momentarily detecting the polarized light reflectance of the sensing surface. While the reflectance in the sensing surface preferably is internal, *i.e.*, the light enters from a dielectric medium of a higher refractive index towards a dielectric medium of a lower refractive index, the reflectance may also be external, *i.e.*, the probing light passes through a layer, such as a sample layer, to be probed on the sensor surface, *e.g.*, external Brewster angle reflectometry and external ellipsometry.

Hereinafter, the present invention will be described in more detail, by way of example only, with regard to some embodiments of the invention. Reference is made to the accompanying drawings, wherein identical parts throughout the Figures are indicated by the same reference designations.

# BRIEF DESCRIPTION OF THE DRAWINGS

Figure 1 is a schematic meridian view of an embodiment of an optical sensor apparatus and light ray paths thereof according to the present invention, which embodiment is based on scanning of the angle of the incident light.

5 Figure 2 is another, parallel schematic meridian view of the embodiment shown in Figure 1.

Figure 3 is a schematic enlarged meridian view of a part of the embodiment shown in Figure 1.

10 Figure 4 is a schematic enlarged meridian view of a part of the embodiment shown in Figure 2.

Figure 5 is a schematic enlarged sagittal view of a part of the embodiment shown in Figure 2.

Figure 6 is a schematic sagittal view of a modified design of the embodiment shown in Figure 5.

15 Figure 7 is a schematic meridian view of the embodiment shown in Figure 6.

Figure 8 is a schematic perspective view of the embodiment shown in Figures 3, 4 and 5.

20 Figure 9 is a schematic perspective view of the embodiment shown in Figure 6.

Figure 10 is a schematic perspective view of a modified design of the embodiment shown in Figure 7.

25 Figure 11 is a schematic exploded view of an alternative embodiment of an optical sensor apparatus and light ray paths thereof according to the present invention, which embodiment is based on scanning of the wavelength of the incident light.

Figure 12 is a schematic enlarged meridian view of a part of a modified version of the embodiment shown in Figure 11.

30 12. Figure 13 a schematic sagittal view of the embodiment shown in Figure

Figure 14 is a schematic meridian view of an alternative embodiment to that shown in Figures 12 and 13.

Figure 15 is a schematic sagittal view of the embodiment shown in Figure 14.

5 Figure 16 is a schematic exploded meridian view of an alternative embodiment of the present invention based on ellipsometry.

Figure 17 is another, parallel, schematic meridian view of the embodiment shown in Figure 16.

10 Figures 18 to 22 are schematic illustrations of prior art means useful for scanning the angle of incident light in apparatuses of the present invention.

Figure 23 is a schematic meridian view of a modified design of the embodiment shown in Figure 2.

Figures 24a to 24d are SPR-images of a sensor surface.

#### DETAILED DESCRIPTION OF THE INVENTION

15 As mentioned above, the present invention relates to an optical method and apparatus for large area or microscopical analysis of structures on a sensor surface, such as real-time monitoring of a chemical sensor or biosensor surface. Usually, the sensor surface has a plurality of individual subzones or areas at which different interactions may take place and produce thin layer structures of optical thicknesses that

20 differ between the subzones. Such "multi-spot" surfaces may be used for a variety of analytical purposes. For example, a surface supporting different ligands on the surface may be subjected to a sample which may contain one or more species, or analytes, capable of binding to respective ligands on the surface. Thereby a sample may be analyzed for the presence of several analyses "in one shot". Other examples and uses

25 are readily apparent to the skilled person.

According to the invention, the sensor surface in question is subjected to illumination with, usually, collimated light on a mainly constant illuminated area and area position, and both image and angle of incidence, and in an alternative form where more than one wavelength is sequentially incident, also wavelength, are simultaneously

monitored by use of the same or another multichannel photodetector or matrix photodetector array than that used for the imaging. A characteristic feature of the invention is that a (usually minor) part of the angular or wavelength-scanned light that illuminates the sensor area for imaging purposes is used to determine the momentary  
 5 incident angle or wavelength of the light. In that way, the momentary incident light angle or wavelength may be directly correlated with the simultaneously produced momentary image of the sensor surface, permitting convenient quantification of the surface subzones where, e.g., a surface binding interaction has taken or takes place.

Figure 1 schematically shows a total internal reflection-based  
 10 embodiment of optical system and ray path according to the present invention, which for the purpose of illustration only is assumed to be a biosensor, for example, of the type described in US-A-5,313,264 and in Jonsson, U., et al., BioTechniques 11:620-627 (1991).

In the system of Figure 1, a light source, LS, illuminates a collimator  
 15 optics, CO, to produce a parallel light beam which passes an interference filter, I, as a monochromatic beam and impinges on a first flat scanner mirror, SM1 to be deflected onto a second scanning mirror, SM2. The latter deflects the beam into a means for coupling the light to a sensor surface, SS. In the illustrated case, this coupling means is a prism, Pr, but may also be a grating as is well known in the art.

20 The sensor surface may be any of a variety of sensor surfaces (which are known or will be known in the future) and, while its basic material structure largely depends on the optical detection principle used, it usually comprises an outer reactive layer, for example having different specific reactive ligands, e.g., antibodies, antigens, nucleic acid fragments, cells or cell fragments, etc., immobilized on defined subzones.  
 25 An exemplary biosensor element for SPR is described in EP-A-442922, whereas exemplary reactive biosensor surfaces are described in US-A-5,242,828 and US-A-5,436,161. The latter comprise a hydrogel (for SPR purposes bound to a gold or silver film), such as dextran, which supports or is capable of covalently binding ligands for reaction with sample analytes.

The sensor surface may further be based on biophysical reactions, where the specific sample interaction results in a structural change manifested as a change in the thickness/refractive index distribution, including absorption, of the sensor layer. Such biophysical interactions include, for example, protein crystallization, formation of protein aggregates caused by precipitation, agglutination or flocculation reactions; the adhesion of membrane complexes, such as biological cells and cell membrane fragments. For further details on the detection of biophysical interactions on a sensor surface it is referred to our copending international application PCT/SE96/01074.

While the sensor surface may be constructed directly on prism Pr in Figure 1, the system described in US-A-5,313,264, referred to above, uses an elastic optical interface ("optointerface") for coupling the light between the prism and the sensor surface. Exemplary optical interface designs are described in US-A-5,164,589 and our copending international application No. PCT/SE96/01522.

The sensor surface is (in the illustrated case) assumed to be exposed on its upper side to a sample containing analyses. The sample may advantageously be contacted with the sample in a flow type cell, e.g., as described in the aforementioned US-A-5,313,264 where one or more flow cells are defined by the sensor surface being docked against one or more open channels in a fluidic block or cartridge.

With reference again to the ray path in Figure 1, the beam is totally internally reflected at the sensor interface side of the coupling prism. The p-polarized component of the beam then passes a polarizer, P, and a main first part of the beam is directed into a first main part of an objective, which main part consists of a spherical objective, SO, producing a real image on matrix detector array, D, of the light intensity reflected from the sensor surface area. The detector array D is arranged such that the real image of the sensor area is produced on a first rectangular main part, D1, of the array. That is, the first part, SO, of the objective has its real image plane positioned at the plane of the photodetector array. Figures 1, 2 and 3 at the detector array D denote the respective images of the corresponding subzones on the sensor surface SS, indicated at 1', 2' and 3', respectively.

The two scanning mirrors, SM1 and SM2, have a related rotational movement which produces an angularly scanned collimated beam incident within a range of angles of incidence on the sensor surface side of the prism Pr. As is readily appreciated by the skilled person, the "beam walk" of the illuminated area may be  
 5 reduced by a suitable choice of the distances between mirrors and prism, and scanned angular range of the mirrors.

Whereas only the above-mentioned first part of the objective is shown in Figure 1, the remaining or second part of it is shown in Figure 2, which is a meridian view of the optical biosensor system parallel to that in Figure 1 and illustrates how the  
 10 ray path for a second minor part of the beam is directed into the second, minor part of the objective consisting of the spherical objective SO, mentioned above, combined with two cylindrical lenses, CL1 and CL2. The latter combination creates a projection of these rays so that the collimated beam reflected at angles within the scanned range is focused onto a second linear minor part D2 of the detector area, separated from the  
 15 detector area used for real image monitoring, so that each angle of reflectance corresponds to a specific detector position within this detector area. That is, the second part of the objective has its back focal plane positioned at the plane of the photodetector array. The letters a, b and c at the detector array D2 indicate the positions on the back focal plane of the focused beams a', b' and c', respectively, which exit the prism Pr, the  
 20 three different angles sequentially illuminating the whole sensor surface and representing three different successive angles of the incident light beam.

The meridian bifocal imaging system described above (one focal length for monitoring the real image, another focal length for monitoring the angle of incidence) enables a simultaneous monitoring of both the position of a reaction site  
 25 within the sensor area (real imaging), and of the quantitative measure of the amount of reacting species (analytes) at the site, by use of the same detector array.

In Figures 1 and 2, the inclined detector plane and the inclined coupling prism exit (non-orthogonal ray-passage at the exit of the prism) indicate the principle, known to anyone skilled in art, to reduce the defocusing of the image at inclined  
 30 imaging.



As already mentioned above, the coupling prism Pr may be replaced by a coupling grating (see, e.g., WO 88/07202 and PCT/GB91/01573).

A more detailed description of the coupling prism, sensor surface, and bifocal imaging system for a combined image- and angle monitoring at the same  
5 detector array is shown in Figures 3 to 10.

Figure 3 (which corresponds to Figure 1) shows a meridian section of ray bundles reflected at different points or sensor zone heights of the sensor surface, indicated at 1', 2' and 3'. Sensor zone heights 1', 2' and 3' are sharply imaged by the spherical objective SO at meridional heights 1, 2 and 3 on the real image plane on the  
10 detector array. For these rays passing only the spherical objective SO, the detector plane is positioned at the real image plane of the lens system.

Figure 4 (which corresponds to Figure 2) shows a meridian section of ray bundles reflected at different angles  $a'$ ,  $b'$ , and  $c'$ , at the sensor surface sagittal height  $O'$  (see Figure 5). Rays reflected at each specific angle are sharply focused to a line at  
15 meridional positions a, b, and c, on the detector D2, by the combined spherical objective and cylindrical elements. For a specific angle of incidence of the collimated light, all the rays will be focused to a line across the columns of detector element designated to angular monitoring. By determining the position of this light intensity peak along such a column, using a suitable algorithm and an angular calibration procedure, a real-time  
20 measurement of the angle of incidence for the related sensor surface 2-dimensional image is enabled with high resolution, accuracy and speed.

Depending on the chosen angular range, an aperture stop,  $A_p$ , may be used to select the rays, and thereby the length along the surface sagittal height  $O'$ , required for angular detection.

25 By introducing an obscuration in a part of the collimated beam, an aperture can be formed in the obscuration for passing of rays used for monitoring of angle of incidence, whereby the width and length of the focused spot or line of these rays at the back focal plane can be suitably adjusted in relation to the size of the pixel and the pixel-separation in the pixel-array of the photodetector, or in the case of a spot-  
30 position sensitive large area sensor, in relation to its area. As such, the number of

pixels, or the area of the photodetector, covered by the spot-intensity peak-width can be optimized for providing a high spot-position resolution, enabling a high sensitivity of measured angle of incidence. As described in Figures 2, 4 and 5, this collimated beam passing the aperture is internally reflected at O', passes lenses CL1 and CL2, and meets the detector plane D2 at O.

The obscuration may be made of any mainly non-transparent material of suitable opto-mechanical properties. The obscuration may be positioned at or within the illumination system, or between the illumination system and the first scanning component. In a preferred embodiment, said obscuration is positioned at the interference filter I, as illustrated in Figure 23.

The aperture is an unobscured opening, taking the shape of a circle, quadrant, or rectangle. The aperture may be positioned either within, or at the edge of the obscuration.

In a preferred embodiment, the aperture is co-centric with the center of the illumination system in the plane of incidence, as shown in Figure 23, while having its center decentered in relation to the illumination system in the direction orthogonal to the plane of incidence, so that the obscuration covers a minor area of the collimated beam that leaves the lens system CO, and the image of the obscuration covers 2-10% of the common photodetector area.

The aperture, has a typical width, in the direction of the plane of incidence, ranging from 0.05-1 mm, a preferred width being 0.2 - 0.5 mm. In case of the aperture taking the form of a rectangular slit, the slit length is typically within 0.5 - 3 mm, a preferred length being 1 - 2 mm.

A suitable masking of the sensor surface at sagittal height O' to limit the reflection area, and/or a suitable structure that always gives total reflection at the sagittal height part O' of the sensor surface may be used to obtain the necessary stability of the intensity peak used for angle determination. This may, for example, be accomplished by a sensor surface which in addition to reactant zones also comprises a part (O') which exhibits a mainly constant reflectance independently of incident angle and wavelength and which thus, in for example SPR, does not give rise to a resonance.

A sagittal section of ray bundles reflected at different parts of the sensor surface is illustrated in Figure 5. Sensor zone heights 4', 5', 6', and 7' are sharply imaged by the spherical objective at sagittal heights 4, 5, 6, and 7 at the detector plane, D, while rays reflected at sagittal height 0' also pass two cylindrical lens elements, CL1 and CL2, which create a defocused intersection of the rays at the detector plane at sagittal position 0. A detector window is indicated at W.

The two cylindrical lens elements may, in the sagittal plane, have a suitable radius, R, providing a refraction in order to locate the image plane of the rays in front of the detector plane, thereby creating a defocusing of the rays across several detector columns used for the angular detection.

Figure 6 shows a sagittal section of an alternative optical system design, wherein the rays used for measuring the angle of incidence are given a suitable ray path folding via two fixed mirrors M1 and M2.

Figure 7 shows a meridian section of another optical design, similar to that in Figure 6, which provides for the ray path folding via two fixed mirrors M1 and M2 in order to obtain a required degree of overlap of the back focal plane and the detector plane within a large angular dynamic range.

The objective and detector design shown in Figures 3 to 5 is schematically represented in a perspective view in Figure 8. Corresponding (schematic) perspective views of the designs shown in Figures 6 and 7 are illustrated in Figures 9 and 10, respectively. Thus, the optical function of monitoring both the real image and the angle of incidence at the same detector array, by use of the above-mentioned first and second parts of the objective, respectively, is depicted in Figure 8, whereas Figure 9 depicts the beam deflection by the folding mirrors M1 and M2 in accordance with the design shown in sagittal view in Figure 6, and in meridian view in Figure 7.

An alternative optical biosensor system according to the present invention based upon wavelength scanning rather than scanning of the incident light angle is shown in Figure 11. To this end the system comprises a scanning monochromator light source, and a wavelength monitoring device.

As previously, the biosensor system comprises a light source, LS, and a collimator optics, CO, to produce a parallel beam, which passes a monochromator, M, and is then directed into a coupling prism Pr (grating coupling is also possible). The collimated beam at a fixed angle of incidence is totally internally reflected at the sensor interface side of the coupling prism. The p-polarized component of the beam then passes a polarizer, P, and is cylindrically focused by lenses, L3 onto a slit, S.

As in the embodiments based on angular scanning above, a minor part of the beam is directed into the minor part of an objective, which minor part consists of a spherical objective, SO, combined with cylindrical lenses, L3 and L4, which create a collimated beam impinging on a transmission grating, T.

The light beam is then dispersed by the grating T so that the direction of propagation of the collimated beam depends upon its wavelength. This beam is then brought to a focus by a cylindrical lens, L5 (alternatively, a mirror in a folded configuration), so that for a scanned wavelength, a spectrum consisting of a series of monochromatic images,  $\lambda_1$ ,  $\lambda_2$ , and  $\lambda_3$  of the entrance slit S at the above-mentioned linear minor area part of a two-dimensional detector array, D2, so that each reflected wavelength corresponds to a specific detector position within this detector area.

For a specific wavelength of incidence of the collimated light, all the dispersed rays will be focused to a line across the columns of detector elements designated to wavelength monitoring. By determining the position of the light intensity peak along such a column, using a suitable algorithm and a wavelength calibration procedure, a real-time measurement of the wavelength of incidence for the related sensor surface (2-D) image is enabled with high accuracy and sensitivity.

As described above for the embodiments using angular scan, one may use a suitable masking at one side of the sensor surface (0' in Figure 13) to limit the reflection area, and/or a suitable, always totally reflecting structure at that sensor surface part to obtain a necessary constancy of the intensity peak used for wavelength determination.

In accordance with the description above for the embodiments using angular scanning, one may also introduce an obscuration in a part of the collimated

beam, wherein an aperture can be formed in the obscuration for passing of rays used for monitoring of wavelength of incidence, whereby the width and length of the focused line at the back focal plane of these rays can be suitably adjusted in relation to the size of the pixel and the pixel-separation in the pixel-array of the photodetector, or in the case of a spot-position sensitive large area sensor, in relation to its area. As such, the number of pixels, or the area of the photodetector, covered by the spot-intensity peak-width can be optimized for providing a high spot-position resolution, enabling a high sensitivity of measured wavelength of incidence.

As described in Figure 13, the collimated beam passing the aperture is internally reflected at O', passes lenses L3, L4, and L5, and grating T, reaching the detector plane at O.

The above described wavelength monitoring construction is illustrated in more detail in Figure 12, which shows a meridian section of ray bundles reflected at a fixed angle at the sensor surface. While in the illustrated case, the dispersive element is a transmission grating, T, it may also be a prism. Rays at each specific wavelength  $\lambda_1$ ,  $\lambda_2$  and  $\lambda_3$ , are collimated by the spherical objective, SO, in combination with the cylindrical elements, L3 and L4, diffracted by the grating, T, and sharply focused by another cylindrical lens, L5, to a line at meridional positions  $\lambda_1$ ,  $\lambda_2$ , and  $\lambda_3$ , on the detector, D, via folding mirrors, M1 and M2.

The dispersive element may be in the form of a focusing reflective grating, positioned at M1 or M2, in a design replacing the equivalently functioning transmission grating T and focusing lens L5 in Figure 12.

Figure 13 shows a sagittal section of ray bundles reflected at different parts of the sensor surface, sensor zone positions 4', 5', 6', and 7' being sharply imaged by the spherical objective, SO, at sagittal positions 4, 5, 6, and 7 at the detector plane, while rays reflected at sensor zone position 0' also pass two cylindrical lens elements, L3 and L4, creating a collimated beam incident on the transmission grating, T. The light beam then passes a cylindrical lens, L5, which focuses the diffracted light in the meridional plane, but defocuses it slightly at the ray-detector plane intersection at

sagittal height 0. For the rays passing only the spherical objective SO, the detector plane is positioned at the real image plane of the lens system.

An alternative embodiment is shown in Figures 14 (meridional view) and 15 (sagittal view), where the collimated beam is deflected by first and second mirrors, M1 and M2, and then passes the dispersive element, here a transmission grating, T, followed by the focusing lens, L5.

Figures 16 and 17 show an alternative embodiment of the optical biosensor system for ellipsometry. The specific ellipsometer components are shown as a typical ellipsometric set-up, and other ellipsometer configurations are obvious to a person skilled in art.

With reference first to Figure 16, the illustrated biosensor system comprises a light source, LS, and a collimator optics, CO, to produce a parallel beam. The latter passes an interference filter, I, and then, as a monochromatic beam, passes a first linear polarizer, P1. The s-component of the this linearly polarized light is then retarded by a quarter-wave plate, Q, below called compensator, which creates an elliptically polarized light beam, impinging on a first flat scanner mirror, SM1. Mirror SM1 deflects the beam onto a second scanning mirror, SM2, which in turn deflects the beam into a coupling prism, Pr (as before, grating coupling is also possible). The beam is totally internally reflected at the sensor interface side of the coupling prism, and then passes a second polarizer, P2, below called analyzer. A main first part of the beam is directed into a first main part of an objective consisting of a spherical objective, SO, producing a real image on a first rectangular main area part a detector array, D, of the light intensity reflected from the sensor area.

In an alternative embodiment, the linear polarizer P1 followed by the compensator are positioned between the mirror SM2 and the prism Pr. For a suitable rotation of both the polarizer and analyzer, at a suitable set-up of orientation of the compensator, angle and wavelength of incidence, the light reflected from a sensor zone can be extinguished. Upon a change in the refractive index or thickness of the sample in the zone, the extinction can be followed by scanning the angle and/or wavelength of incidence.

Figure 17 shows a meridian view of the optical biosensor system, parallel to the view in Figure 16. Here the ray path for a second, minor part of the beam is directed into a second, minor part of the objective consisting of the spherical objective, SO, combined with two cylindrical lenses, CL1 and CL2. This lens combination creates a projection of these rays so that the collimated beam reflected at different angles, here represented by beams a', b' and c', within the scanned range is focused onto a second linear minor part of the detector area, at a, b and c, respectively, this detector area being separated from the detector area used for real image monitoring, so that each angle of reflectance will correspond to a specific detector position within this detector area. Thus, the above-mentioned second part of the objective has its back focal plane positioned at the plane of the photodetector array.

The above described meridian bifocal imaging system in combination with an ellipsometer provides a simultaneous monitoring of both the position of a reaction site within the sensor area (real imaging), and of the quantitative measure of the amount of reacting species at the site, via at least one of the angle or wavelength of incidence, by use of the same detector array.

From the above description of exemplary optical system designs embodying the present invention it is readily seen that monitoring the actual change of at least one of the angle and wavelength of incidence via the bifocal imaging represents a considerable advantage in relation to the prior art in that the need to derive this change from any steering signal driving the angle scanner or scanning monochromator is eliminated. The scanner driver electronics and software thus just have to provide a suitable dynamic range and scan speed for the angle or wavelength.

The above described optical designs demonstrate the optical function of the present invention. It is, however, readily appreciated by a person skilled in the art, that these optical designs could be optimized to achieve a suitable performance and function of an apparatus constructed based on these designs.

Also, while in the above described optical systems the bifocal (in the meridian plane) imaging system is based on lens optics, it is readily understood that the imaging system may comprise diffractive optical surfaces for improving imaging

quality, image plane flatness, and image plane tilt, to match the needs of the photodetector array. Furthermore, diffractive optics may be the main component in the objective which forms the above described real image and angular projection on two separate areas of the same detector array.

5 In the following, the different parts of apparatus embodying the above described optical functions will be described in more detail.

Thus, in accordance with the embodiments of Figures 1 to 10 described above, the optical construction employs an illumination system comprising a mainly monochromatic light source and a scanning plane mirror system, an optical coupling  
10 component (plane sided prism or grating) in optical contact with a sensing surface, an imaging system comprising a bifocal objective and a photodetector matrix array. An algorithm and a computer program are provided which permit an interpretation of the signals from a first main part of the photodetector into a real image of the sensor pattern, and from a second minor part of the photodetector into the angle of incidence of  
15 the probing light. The angle of incidence at a specific parameter of the light intensity, e.g., minimum or maximum, for each sensor zone may thus be monitored simultaneously.

For example, the invention permits a beam having a diameter within the range of about 3 mm to 30 mm to be angularly or wavelength scanned and monitored at  
20 a resolution of 0.0001 degrees, and 0.002 nm, respectively, within the range of angle or wavelength of interest, wherein the rays are collimated to a required degree (preferably within about 0.002 degrees).

#### Illumination system

The illumination system creates a collimated beam at a suitable  
25 monochromatic wavelength. In the angular scan mode of the invention, the beam is scanned by a plane mirror system creating a collimated beam, the angle of incidence of which at the sensing surface is scanned while the illuminated area at the sensing surface is mainly fixed. In the wavelength scan mode, a wavelength dispersive device in



combination with collimator optics create a collimated beam which is incident at the sensing surface at a fixed angle.

The light incident on the total internal reflection interface may be p-polarized or consist of both p- and s-polarized components, *i.e.*, being suitably  
5 elliptically polarized.

The light source may be either mainly non-coherent, *e.g.*, a light emitting diode, a tungsten-halogen lamp, or mainly coherent, *e.g.*, a laser diode.

In an apparatus based on angular scanning, the light source may be either mainly monochromatic, *e.g.*, a light emitting diode in combination with an interference  
10 filter, or a laser diode, or a light source capable of sequentially emitting a suitable number of wavelengths, one specific wavelength at each angular scan.

In an apparatus based on wavelength scanning, the light source may, *e.g.*, be a white light source, such as a tungsten-halogen lamp, in combination with a scanning wavelength dispersive device. Such a scanning monochromator may be  
15 motorized to sequentially emit wavelengths within a wavelength range, which in combination with the collimator creates a collimated beam.

#### Angle scanning means

Fundamentally, scanning devices are light beam deflectors. Deflectors can be categorized into reflective, refractive, and diffractive (acousto-optic scanners, holographic scanners). Scan patterns and scanning motions are inextricably interrelated  
20 involving both beam displacement and beam-displacement rate, and beam deflection and beam-deflection rate. Scanning motions essentially fall into three basic movements, rotational, oscillatory, and translational.

The scanning of the angle of incidence with time of a parallel light beam  
25 by utilizing a collimated beam deflecting element, may be created by low inertia components, *e.g.*, vibrating or rotating mirrors or a moving grating, or an inertialess acousto-optical deflector.

The beam deflecting system for an angularly scanned imaging consists in a preferred embodiment of mirrors, which as non-refractive optics does not need to be

corrected for chromatic aberrations. In a preferred form, two oscillating or rotating inter-related plane mirrors are combined with a plane sided coupling prism, or a grating, which deflects a collimated beam during the angular scan of the beam so that the optical axis of the beam always intersects mainly the same point at the sensor surface (to obtain  
 5 reduced beam walking, *i.e.*, improved stability of the light intensity which improves the sensitivity of the instrument), and an imaging system designed to create a real image of the sensor surface in combination with a simultaneous projection of the reflected light into an instant measure of the actual angle of incidence.

The incident angle for collimated beams should typically be scanned  
 10 within an angular range of  $\pm 5^\circ$ , with a detected angular resolution of  $\leq 0.0001^\circ$ , corresponding to a refractive index resolution of 0.000001. For real-time monitoring, the angular scan should be rapid.

A preferred scanned angular interval is  $\approx 70 \pm 6^\circ$  at a wavelength of 820 nm, alternatively,  $\approx 77 \pm 8^\circ$  at a wavelength of 660 nm.

15 The bifocal imaging system described above, may be combined with any of the numerous arrangements for angular scanning of a collimated incident beam available in the literature.

A preferred angular scanner comprising two plane mirrors, the turning movements of which are interrelated via the steering electronics, has already been  
 20 described in connection with Figures 1 and 2.

A first alternative scanning principle is the twin parallel-mirror described in Harrick, N.J., Internal Reflection Spectroscopy, Harrick Scientific Corp., 1987, New York, p. 185, and shown in Figure 18 herein, however, after replacing the convex coupling lens in Figure 18 with a prism as in the specifically described embodiments of  
 25 the present invention.

A second alternative scanning principle is an optically optimized (*i.e.*, to obtain overlapping focal surfaces for the whole angular range) system comprising one plane mirror and focal surface flattening optics, in accordance with the scanners described by Lenferink, A.T.M. et al., Sensors and Actuators B, 3 (1991) p. 262, shown

in Figure 19 herein, and Oda, K., et al., Optics Communications, Vol. 59, No. 5, 6, 1986, p. 362, shown in Figure 20 herein.

Still another alternative scanning principle, equivalent to the previous one for focal surface flattening optics, consists of a plane mirror, SM1, scanning a  
 5 focused beam from the illumination source, LS, along a focal surface of a concave mirror, Mc, creating an angle scanned collimated beam, as shown in Figure 21. This may also be described as that the illumination system includes one oscillating/or rotating plane mirror in combination with a concave cylindrical mirror, which deflects a focused beam during the angular scan of the beam so that its focal surface overlaps the  
 10 focal surface of the cylindrical mirror, thereby creating a scanning collimated beam.

Still another alternative scanning principle comprises a pivotally moving illumination system, e.g., such as that described in WO 93/14392, and shown in Figure 22 herein.

Still another possible scanning structure is an excentric rotating  
 15 polygonic scanner, replacing the cooperating mirrors SM1 and SM2 in Figures 1 and 2. Typically, such a polygonic scanner consists of eight planar mirrors mounted on the periphery of a rotating wheel.

#### Wavelength scanning means

When the reflectometry in the method and apparatus of the present  
 20 invention is performed as a function of the incident wavelength at a fixed angle, the light source is combined with a scanning monochromator which in combination with the real imaging and image detection sequentially creates a series of images, each of a specific wavelength. A smaller part of the same image detector (or a separate detector) is used for measuring the wavelength. For this dual detector function to be possible,  
 25 this smaller detector part is combined with a wavelength dispersive element, which spatially separates light at different wavelengths.

The incident wavelength should typically be scanned within a wavelength range of  $\pm 200$  nm, with a detected wavelength resolution of  $\leq 0.002$  nm, corresponding to a refractive index resolution of 0.000001.

In its simplest form, the dispersive element consists of a prism. Due to the refraction of the light in the prism, the rays must be deflected by, *e.g.*, a reflective element, in order to reach the detector.

A grating spectrograph is similar to a prism spectrograph. The light to be analyzed passes first through a combination of a slit and a collimating lens. It then reaches the reflecting or transmission grating, set with its grooves parallel to the slit, where light of different wavelengths is diffracted at different angles, and is for each order drawn out into a spectrum. A second lens focuses these diffracted rays onto the detector array. A grating with a high groove density per unit width may give a few orders, but their spectra are spread out much wider than those formed by a lower density.

Generally, as is understood by the skilled person, the bifocal imaging system described above with the specific embodiments of the biosensor system of the invention may be combined with numerous arrangements for scanning monochromators available in the literature.

#### Sensor surface and opto-coupling to the collimated beam

In a preferred embodiment, the collimated light impinges on the interface between sensor surface substrate and the actual sensor surface under total internal reflection conditions. The substrate/sensor surface may be a separate exchangeable component consisting of a sensing layer coating a transparent substrate, *e.g.*, of glass or plastic, that is in optical contact with the optical coupling media described above. The substrate should be matched in respect of refractive index to a coupling prism which transmits the light beams of the illumination system to the sensor surface. Alternatively, a plane side of the coupling prism may be the substrate.

According to an alternative opto-coupling principle, the substrate may be in the form of a grating on either the sensor surface substrate interface, or on the opposite side to this interface on the substrate.

When, for example, the detection principle is based on SPR, the sensor surface comprises a plasmon-active material, such as gold or silver. In the case of

internal Brewster angle detection, on the other hand, the sensor surface is of a transparent material, *i.e.*, there is no metal film.

The sensor surface part at the sensor surface plane that provides the light for the detection of angle or wavelength should have a low variation in reflectance for the scanned angle/wavelength range. A varying light intensity during the scan mode of the invention, *e.g.*, as caused by SPR also within this part of the detected light, is likely to disturb the accuracy of the angular determination. It is therefore preferred to use for the angle/wavelength measurement a part of the sensor surface that is not brought in contact with the sample, *e.g.*, a part in contact with flow cell material in case of a sensor surface docking system of the type described in the aforementioned US-A-5,313,264. Such a part may be located, *e.g.*, at the flow cell wall, by the software used in the instrument. Thereby, the light intensity of the focused line on the detector will be insensitive to any light interaction with the sample during the angular or wavelength scan.

Alternatively, a purely reflecting part (no evanescent wave) of the sensor chip is used for the measurement of the incident light angle or wavelength to obtain a light beam intensity during the angular or wavelength scan that is not influenced by the sample.

#### Imaging system

Depending on the choice of microscopy monitoring or degree of large area monitoring, the person skilled in art may design a suitable imaging system.

In the case of angular scanning, for each specific incident angle the reflected light is collected by an objective, which images a mainly stationarily illuminated sensor area. A possible marginal walk of the illuminated area is not a problem, provided that it is the stationarily illuminated central part of the illuminated sensor surface that is imaged. The imaging system creates an image in the detector plane where the reflectance minima or maxima correspond to the local distribution of refractive index over the sample area. An optimum light intensity for imaging requires

that the main part of the illuminating optical power is localized to the stationarily illuminated and imaging part of the sensor surface.

For microscopy applications, the sensor area is enlarged, typically 20-40X. This image may be detected by a photodetector matrix, *e.g.*, of CCD (charged coupled device) camera type. Alternatively, this image may be further enlarged by an

ocular, typically 10-20X, and projected on the photodetector matrix.

For large area applications, the sensor surface is generally reduced. Typically, a sensor area of, say, 3 cm x 3 cm is reduced about 0.3X - 0.6X on a conventional CCD-detector.

Two exemplary designs of imaging systems for use in the present invention are given below:

1. An objective of magnification 15X together with a photodetector array with pixel dimensions  $15 \times 15 \mu\text{m}^2$ , and an array-area of  $6 \times 8 \text{ mm}^2$ , may monitor a total sensor area of approximately  $0.4 \times 0.5 \text{ mm}^2$  with a lateral resolution of  $1 \times 1 \mu\text{m}^2$ .
2. An objective of magnification 0.2X with pixel dimensions  $15 \times 15 \mu\text{m}^2$ , and an array area of  $6 \times 8 \text{ mm}^2$ , may monitor a total sensor area of approximately  $3 \times 4 \text{ cm}^2$  with a lateral resolution of  $75 \times 75 \mu\text{m}^2$ .

#### Image processing and monitoring software

An outline of the requirements on the computer software for the analysis and presentation of the monitored reaction zones is given below.

By the use of non-coherent light, the distribution of totally internally reflected reflectance minima over the sensor surface may be detected in the form of images synchronized to the incident angle of the illuminating light. The image reflectance data and image-related data are processed in real-time in an image processing computer program to provide, for example, a three-dimensional refractometric image with the quantified mass-distribution as a function of sensor surface coordinate.

A high time resolution between the refractometric images requires a short angle-scanning period. A typical commercially interesting frame-rate range is of

the order of 50-60 Hz. Each frame of detected intensity corresponds to a specific angle or wavelength. Thus, during one second a number of 50-60 intensity- and angle-data points are read for each of the detector elements corresponding to a sensor zone.

To obtain a suitable mean value for a cluster of detector elements covering a specific sensor zone, the image processing software calculates a reflectance curve for the zone by first averaging the intensity of the chosen elements at each angle or wavelength, and then plots this intensity versus the angle or wavelength. For example, each zone may obtain one reflectance curve per second (*i.e.*, the reflectance curve rate is 1 Hz). A second algorithm calculates the angle or wavelength at the curve parameter correlated to the refractive index within the sampled zone, normally, the minimum reflectance or centroid of the dip in the reflectance curve.

The higher the rate of the sample interaction with the sensor zone, the higher angle and/or wavelength resolution is required, and the higher frame rate will be needed for the image processing.

The real image on a first main part of the matrix detector is read and stored by a so-called frame-grabbing program, while the position of maximum intensity, or alternatively, the centroid of the intensity curve, for the angle- or wavelength-related beams focused on a second minor part of the detector matrix is calculated and stored by a suitable algorithm.

An exemplary measurement/calculation procedure based on the angular scan mode is described below.

First, an initial normalization of reflectance data is performed by measuring total reflectance during an angular scan without sample addition. This procedure may comprise the following steps:

- a) Define for each sensor zone a cluster of pixels on the photodetector matrix, including a center pixel and a selected number of neighboring pixels,
- b) start a clock for the measurement process,

c) start driving an angle scan over a predetermined angular range (driving is, e.g., stepping or rotational motor control or moving coil current for oscillating mirrors),

d) read from the 2-D image detector part of the photodetector matrix  
5 into an image data memory, a sequence of raw data images for averaged 2-D reflectance from the detector pixels corresponding to each sensor surface zone,

e) simultaneously, read from the angle detector pixel row of the photodetector to an angular data memory, a sequence of raw data for the reflectance intensity peak (pixel number, time),

10 f) calculate for each 2-D image the incident angle from the pixel number of the respective intensity peak on the detector pixel row,

g) store the angle and time for the respective raw data images in an image/angle/time matrix,

15 h) calculate a normalizing matrix from the measured reflectance values of the 2-D image, the normalized reflectance being identical within the sensor zones for all angles, and

i) store a normalizing matrix (normalizing data, angle).

The system is now ready for monitoring sample surface concentrations at each sensor zone by measuring reflectance minima during the angular scan.

20 Measurements are performed first with only solvent at the surface and then with sample plus solvent. The measurement procedure may comprise the following steps:

a) start a clock for the measurement process,

b) start driving an angle scan over a predetermined angular range,

c) read from the 2-D image detector part of the photodetector matrix  
25 into an image data memory, a sequence of raw data for averaged 2-D reflectance images from the detector pixels corresponding to each sensor surface zone,

d) simultaneously read from the angle detector pixel row or rows of the photodetector to an angular data memory, a sequence of raw data for the reflectance intensity peak (pixel number, time),



- e) calculate for each 2-D image the incident angle from the pixel number of the respective intensity peak on the detector pixel row,
- f) store the angle and time for the respective images in an image/angle/time matrix,
- 5 g) calculate a normalized 2-D image from the raw data matrix of the 2-D image by correcting with the respective normalizing matrix,
- h) store the angle and time for the respective normalized image in a normalized image/angle/time matrix,
- i) select a specific sensor zone and the corresponding part of the
- 10 normalized image/angle/time matrix,
- j) copy data for the angular dependence of the reflectance curve (normalized reflectance, angle),
- k) calculate from the data in j) the angle and reflectance of the reflectance minimum,
- 15 l) calculate from the normalized reflectance matrix a medium time for the angular scan  $((\text{start time} + \text{stop time})/2)$ ,
- m) store a medium time for the reflectance minimum angle (in k)) and the specific sensor zone in a reflectance minimum angle/sensor zone/medium time matrix,
- 20 n) calculate the reflectance minimum angle shift for the respective sensor zone and time in relation to a reference angle for the sensor zone obtained before the sample reaction therewith,
- o) calculate from the angle shift the internal surface concentration of the sensor zone,
- 25 p) store the internal surface concentration in a matrix (surface concentration, medium time),
- q) select the next specific sensor surface zone and calculate the surface concentration as above,
- r) calculate a differential surface concentration for selected
- 30 reference zones,

s) store the relative surface concentration in a matrix (differential surface concentration, medium time),

t) present simultaneously in graphs or tables the internal and relative surface concentrations, respectively, as a function of time for the respective  
5 surface zone,

u) start the driving of the next angular scan, and

v) repeat the above measuring procedure up to a final analysis time.

The driving of the angle may be continuous and the storing of the image and angle data may be triggered by the angle data scanning over the predetermined  
10 angular range. These stored image/angle/time-matrices are shifted into the calculation and presentation procedures at a rate depending on the computer performance.

Instead of measuring and presenting surface concentrations, it is, of course, possible to measure and present surface concentration changes, surface refractive indexes, surface refractive index changes, surface thicknesses and surface  
15 thickness changes.

The amounts of sample species bound or adsorbed to the different sensor spots or subzones may be related to each other by analytical software. The time relation of the refractometric images makes it possible to obtain via further image data processing mass distribution kinetic data for, e.g., specific sample binding/desorption,  
20 sample displacement along the sensor surface, or for the separation process.

The use of coherent light makes it possible to detect, in addition to the distribution of total internal reflectance minima over the sensor surface, also interferometric changes caused by locally changed mass distributions. Image data processing of the lateral movement pattern of such interference bands may be used to  
25 obtain an increased sensitivity to lateral refractive index changes on the sensor surface.



### Experimental Procedure Example

The principle of the present invention was verified as demonstrated in Figures 24a - 24d, by use of a pivotally moving illumination system similar to the one described in Figure 22, using a light emitting diode of center-wavelength 766 nm, lenses and a sheet-polarizer providing p-polarized collimated beam of diameter 8 mm, an interference filter of bandwidth 3 nm, an imaging embodiment according to Figures 3, 4, and 5, and a CCD-photodetector matrix connected to a video-recorder. The obscuration, imaged as the dark right part in Figures 24a - 24d covering about 25% of the image, is positioned at the interference filter I, Figure 23, decentered in relation to the beam cross-section, so that it covers about 15% of the beam width.

Figures 24a - 24d show a series of SPR-images of a sensor surface exposed to rinse solution in a flow cell, the sensor surface consisting of sixteen zones of various refractive index (optical thickness), zone size 0.5 mm x 0.5 mm, each image at a specific angle of incidence increasing in the order from a) to d). The lower the position of the focused spot within the angle-detecting area of the CCD, the larger is the angle of incidence. The angle of incidence is 65.9° in Figure 24a, 66.4° in Figure 24b, 66.9° in Figure 24c, and 67.4° in Figure 24d.

Since a change in the angle for SPR of 0.1° here corresponds to a change in the refractive index of 0.001 within the zone's reactive layer, the shift in refractive index is 0.005 between Figures 24a and 24b, 24b and 24c, and 24c and 24d, respectively.

At SPR within a specific zone, detected as a minimum of light reflected in the zone, the corresponding angle of incidence is a measure of the refractive index (optical thickness) of the zone. The larger the angle of incidence at SPR is, the larger is the optical thickness (or refractive index at fixed thickness), which corresponds to a larger surface concentration of bound sample to a zone.

In Figure 24a the following zone-coordinates (row, column) show light extinction due to SPR: (1,1), (1,2), (1,3), which the higher angle of incidence in Figure 24b causes SPR in the zones: (2,1), (2,2), (3,1), (3,2), revealing a higher surface concentration in the latter zones. In Figure 24c, the zones of the sensor surface having

yet higher surface concentration of sample are revealed in zones (4,2) and (4,3). In Figure 24d, the zone of the sensor surface having the highest surface concentration of sample are revealed in zone (4,1).

As an example, the refractive index in zone (3,1) is 0.005 higher than the one for zone (1,1), while the refractive index in zone (4,2) is 0.005 higher than the one for zone (2,1), and the refractive index in zone (4,1) is 0.015 higher than the one for zone (1,1).

The above described results demonstrate the function of the present invention, an optical apparatus for multi-zone quantitative analysis on a sensor surface by use of simultaneous measuring of zone-data and angle-data on the same photodetector matrix. It is then readily appreciated by a person skilled in the art, that a suitable evaluation computer program could provide a high-sensitive and fast determination of the angle for SPR for specific sensor zones by combining a first computer program for one-dimensional spot-position analysis with a second computer program for two-dimensional intensity-pattern analysis.

Furthermore, it is readily appreciated by a person skilled in the art, that the invention also provides for measurement of zone-data on a photodetector matrix and a simultaneous measurement of angle-data on a separate detector.

From the foregoing it will be appreciated that, although specific embodiments of the invention have been described herein for purposes of illustration, various modifications may be made without deviating from the spirit and scope of the invention. Accordingly, the invention is not limited except as by the appended claims.

Throughout this specification and the claims which follow, unless the context requires otherwise, the word "comprise", and variations such as "comprises" and "comprising", will be understood to imply the inclusion of a stated integer or step or group of integers or steps but not the exclusion of any other integer or step or group of integers or steps.

## THE CLAIMS DEFINING THE INVENTION ARE AS FOLLOWS:

1. An optical apparatus for examining thin layer structures on a surface for differences  
 5 in respect of optical thickness, comprising:
- a sensor unit having a sensor surface with a number of zones capable of exhibiting thin layer structures of varying optical thickness, particularly as the result of contact with a sample,
  - a light source for emitting a beam of light,
  - 10 optical means for coupling said light beam to said sensor unit,
  - first photodetector means,
  - means for imaging light reflected from said different parts of the sensor surface onto said first photodetector means for detecting the intensities of the reflected light from the sensor surface,
  - 15 means for sequentially or continuously scanning said light incident at said sensor surface over a range of incident angles and/or wavelengths,
  - means for determining each angle and/or wavelength of light impinging on said sensing surface,
  - evaluation means for determining from the relationship between detected intensity  
 20 of the reflected light and incident light angle and/or wavelength, the optical thickness of each zone of said sensor surface to thereby produce a morphometric image of the optical thickness of the sensor surface,
  - characterised in that the apparatus comprises second photodetector means, and that said means for determining said light angles and/or wavelengths comprise means for  
 25 focusing a part of monochromatic light reflected at the sensing surface onto the second photodetector means, wherein each position of said focused light on said second photodetector means is related to a specific angle and/or wavelength of the light incident at the sensing surface.



2. The apparatus according to claim 1, characterised in that said imaging means to compromise a bifocal lens system comprising a first part having its real image plane at the plane of said first photodetecotor means, and a second part having its back focal plane at the place of said second photodetecor means, so that at the back focal plane the spatial reflectance is transformed to the spatial reflectance angle.

3. The apparatus according to claim 2, characterised in that said first part of the bifocal lens system is a spherical lens system, and that said second part of the bifocal lens system is said spherical lens system combined with a cylindrical lens system.

4. The apparatus according to any preceding claim, characterised in that the apparatus includes a wavelength dispersive element, so that at the back focal plane the spatial reflectance is transformed to the spatially reflected wavelength.

5. The apparatus according to any preceding claim, characterised in that said first and second photodetector means are different parts of a single two-dimensional matrix of photodetector elements.

6. The apparatus according to claim 5 when dependent upon claim 4, characterised in that said photodetector matrix array comprises a first part for imaging the sensing surface, a second part for determining the angle of the incident light, and a third part for determining the wavelength of the incident light.

7. The apparatus according to claim 5 or 6, characterised in that said photodetector matrix array comprises a first main detector area positioned at the image plane of the bifocal lens system, and a second detector area positioned at the back focal plane of the bifocal plane of the bifocal lens system, so that at said first main detector area each detector element via the real image of the sensor surface corresponds to a co-ordinate of the sensor surface, and at said second detector area each detector element via the position of the light corresponds to the angle of incidence.

8. The apparatus according to any one of claims 5 to 7, characterised in that said photodetector matrix array comprises a first main detector area positioned at the image plane of the bifocal lens system, and a second detector area positioned at the back focal plane of the bifocal lens system, so that at said first main detector area each detector element via the real image of the sensor surface corresponds to a co-ordinate of the sensor surface, and at said second detector area each detector element via the positioned of the light corresponds to the wavelength.

9. The apparatus according to any preceding claim, characterised in that said scanning means comprise beam deflecting means to produce an angle-scanned collimated illumination of the sensor surface with a substantially stationary illuminated sensor surface area and area position for a given angular interval, at which sensor area each surface point momentarily is illuminated by light rays of identical angle of incidence and wavelength.

10. The apparatus according to claim 9, characterised in that said beam deflecting means comprise an acousto-optical deflector.

11. The apparatus according to any preceding claim, characterised in that said optical coupling means is either a prism or lens having at least one plane side, or a grating.

12. The apparatus according to any preceding claim, characterised in that said evaluation means comprise an evaluation unit for determining the angle, and/or the wavelength, for minimum reflectance of p-polarised light, and/or the relative reflectance and phase of the p- and s-polarised electric field components of the light for each of the specific multi-zones.

13. The apparatus according to any preceding claim, characterised in that said evaluation means comprise an evaluation unit for calculating and presenting the surface structures for each of the specific multi-zones of the sensing surface.

14. The apparatus according to any preceding claim, characterised in that said sensing supports reactants capable of binding interaction with species in a sample, particularly biomolecules, to produce said thin surface structures to be examined.

15. The apparatus according to any preceding claim, characterised in that the apparatus comprises a sample solution container in contact with the sensor unit to expose the sensing surface to sample solution.

16. The apparatus according to claim 15, characterised in that said sample solution container is a flow cell.

17. The apparatus according to claim 16, characterised in that said sample solution container is a wall-jet flow cell, in which a jet flow is directed orthogonally against said sensing surface.

18. The apparatus according to any preceding claim, characterised in that said angular scanning means comprise two inter-related oscillating mirrors.

19. The apparatus according to any one of claims 1 to 17, characterised in that said scanning means for sequentially or continuously scanning said light incident at said sensor surface comprise two mirrors in a fixed configuration which is oscillated or rotated.

20. The apparatus according to any one of claims 1 to 17, characterised in that said scanning means for sequentially or continuously scanning said light incident at said sensor surface comprise an oscillating plane mirror and a concave mirror.

21. The apparatus according to any one of claims 1 to 17, characterised in that said scanning for sequentially or continuously scanning said light incident at said sensor surface means comprise a translationally moving plane mirror in combination with a generally concave cylindrical fixed mirror.

---



22. The apparatus according to any one of claims 1 to 17, characterised in that said scanning means for sequentially or continuously scanning said light incident at said sensor surface comprise a pivotally moving plane mirror in combination with said optical coupling means.

23. The apparatus according to any one of claims 1 to 17, characterised in that said scanning means for sequentially or continuously scanning said light incident at said sensor surface comprise a rotating polygon plane mirror in combination with said optical coupling means.

24. The apparatus according to any one of claims 1 to 17, characterised in that said scanning means for sequentially or continuously scanning said light incident at said sensor surface comprise two telecentric angular scanners including an oscillating plane mirror and a first focusing optical component, which creates a scanned focal line, said focal line-surface coinciding with the focal line-surface of a second focusing optical component, thus creating a collimated beam of scanned angle of incidence.

25. The apparatus according to claim 24, characterised in that said first and second focusing optical components are convex cylindrical lenses.

26. The apparatus according to claim 24, characterised in that said first focusing component is a convex cylindrical lens, and that said second virtually focusing component is a virtually focusing concave cylindrical lens.

27. The apparatus according to claim 24, characterised in that said first focusing component is a virtually focusing component in the form of a diverging (negative) lens, and the second focusing component is a convex cylindrical lens.

28. The apparatus according to claim 24, characterised in that said scanning means for sequentially or continuously scanning said light incident at said sensor surface comprise a pivotally moving illumination system.

---

29. The apparatus according to any preceding claim, characterised in that said light source emits substantially monochromatic and non-coherent light.

30. The apparatus according to claim 29, characterised in that said light source is a light emitting diode in combination with an interference filter.

31. The apparatus according to any one of claims 1 to 28, characterised in that said light source emits substantially monochromatic and coherent light.

32. The apparatus according to claim 31, characterised in that said light source is a semiconductor diode laser, a dye laser, or a gas laser.

33. The apparatus according to claim 32, characterised in that said beam deflecting means comprise a holographic beam deflector.

34. The apparatus according to any preceding claim, characterised in that said light source emits a continuous light spectrum, and is combined with a scanning monochromator for sequentially providing more than one wavelength.

35. The apparatus according to any preceding claim, characterised in that the plane of said first and second photodetector means is inclined in relation to the plane of reflection, so that the focus plane of real image of the sensor surface coincides with the photodetector plane.

36. The apparatus according to any preceding claim, characterised in that the apparatus comprises a wedge-shaped transparent body that corrects for defocusing refraction at an inclined observing view and within the light coupling element for the range of angle of incidence.

37. The apparatus according to any preceding claim, characterised in that said apparatus is based on determining total internal reflection versus angle and/or wavelength of incidence.

---

- 47 -

38. The apparatus according to Claim 37, characterised in that said internal reflection versus angle and/or wavelength of incidence determination is based upon surface plasmon resonance, Brewster angle, ellipsometry, critical angle, or frustrated total reflection waveguide resonance.

5

39. The apparatus according to any preceding claim, characterised in that said sensor unit is designed to be exchangeable in the apparatus.


40. The apparatus according to any preceding claim, characterised in that said sensor unit is an integral part of said optical coupling means, especially a prism or grating.

10



41. The apparatus according to any preceding claim, characterised in that said sensor unit comprises a first part covered by said sensing surface zones, and a second part providing constant reflectance during the scan of at least one of angle and wavelength of incidence.

15



42. The apparatus according to any preceding claim, characterised in that the apparatus comprises an exchangeable resilient opto-coupling member designed to interface both the sensor unit and said optical coupling means.

20

43. The apparatus according to any one of Claims 1 to 42, characterised in that said evaluation means provides for image processing where a detected coherent light reflectance pattern and interference pattern for the sensor surface is correlated to both the angle of incidence and time to create a four-dimensional real-time refractometric representation of the lateral optical thickness distribution on the sensing surface.

25

44. The apparatus according to any preceding claim, characterised in that said evaluation means provides for image processing where a detected coherent light reflectance pattern and interference pattern for the sensor surface is correlated to both the angle of incidence and/or wavelength and time to create a five-dimensional real-time refractometric representation of the lateral optical thickness distribution as a function of

30



- 48 -

penetration depth of the evanescent wave, created in said total internal reflection, on the sensing surface.

45. The apparatus according to any one of claims 1 to 42, characterised in that said  
5 evaluation means provides for image processing where a detected non-coherent light  
reflectance pattern for the sensor surface is correlated to both the angle of incidence and  
time to create a four-dimensional real-time refractometric representation of the lateral  
optical thickness distribution on the sensing surface.

10  
15

46. The apparatus according to any one of claims 1 to 42, characterised in that said  
evaluation means provides for image processing where a detected non-coherent light  
reflectance pattern for the sensing surface is correlated to both the angle of incidence  
and/or wavelength and time to create a five-dimensional real-time refractometric  
representation of the lateral optical thickness distribution as a function of penetration depth  
15 of an evanescent wave, created in said total internal reflection, on the sensing surface.

20

47. The apparatus according to any preceding claim, characterised in that the apparatus  
comprises computer means.

20 48. The apparatus according to any preceding claim, characterised in that the apparatus  
comprises optical means placed between the light source and the detector for polarising  
said light.



- 49 -

49. The apparatus according to any preceding claim, characterised in that said light source emits polarised light.

50. The apparatus according to any preceding claim, characterised in that said apparatus  
5 comprises at least one aperture in at least one obscuration positioned in at least one part of the beam scanned in at least one of the angles or wavelengths of incidence, for determining the cross-section geometry of the light beam used for monitoring angle and/or wavelength.

51. A method of using an optical apparatus according to any one of claims 1 to 50 for  
10 examining thin layer structures on a surface for differences in respect of optical thickness, which method comprises:

irradiating the surface with light so that the light is internally or externally reflected at the surface,

imaging the reflected light on a first two-dimensional detector,

15 sequentially or continuously scanning the incident angle and/or wavelength of the light over an angular and/or wavelength range,

measuring the intensities of light reflected from different parts of the surface and impinging on different on different parts of the detector, at at least a number of incident angles and/or wavelengths, the intensity of light reflected from each part of the surface for  
20 each angle and/or wavelength depending on the optical thickness of the thin layer structure thereon,

and determining from the detected light intensities at the different light incident angles and/or wavelengths an optical thickness image of the thin layer structures on the surface,

25 characterised in that part of the light reflected at said surface is detected on a second detector to determine the incident angle or wavelength of the polarised light irradiating the surface.

52. The method according to Claim 51, characterised in that said part of the light for determining the incident angle or wavelength is focused on said second detector as a point or line, the position of said point or line on the detector being related to the angle or wavelength of the incident light.

53. The method according to Claim 51 or 52, characterised in that the angle of the incident light is scanned.

54. The method according to Claim 51 or 52, characterised in that the wavelength of the incident light is scanned.

55. The method according to any one of Claims 51 to 54, characterised in that said first and second detectors are different parts of a single photodetector matrix array.

56. The method according to any one of Claims 51 to 55, characterised in that said light is non-coherent.

57. The method according to any one of Claims 51 to 55, characterised in that said light is coherent.

58. The method according to any one of Claims 51 to 57, characterised in that said light is totally internally reflected from said surface.

59. The method according to Claim 58, characterised in that said light is coupled to said surface via a prism or grating.

---

60. The method according to Claim 58 or 59, characterised in that said determination of reflection versus angle and/or wavelength is based on evanescent wave sensing.

61. The method according to Claim 60, characterised in that said determination of reflection versus angle and/or wavelength is based on surface plasmon resonance, Brewster angle, ellipsometry, critical angle or frustrated total reflection waveguide resonance.

62. The method according to any one of Claims 51 to 57, characterised in that said light is externally reflected from said surface.

63. The method according to Claim 62, characterised in that said determination of reflection versus angle and/or wavelength is based on external Brewster angle or external ellipsometry.

64. The method according to any one of Claims 51 to 63, characterised in that said surface is a chemical or biochemical sensor surface having a number of subzones, each subzone supporting a reactant capable of interacting with a specific analyte species, and that said surface is contacted with a sample suspected of containing one or more of said specific analyte species to determine their presence in the sample.

65. The method according to any one of Claims 51 to 64, characterised in that said light used for determining the angle and/or wavelength of the incident light is reflected at a part of said surface that does not exhibit said thin layer structures, especially at a part of said surface that is not contacted by said sample.

---

66. The method according to any one of Claims 51 to 65, characterised in that it comprises determining, based on said thickness images on said surface, at least one of the corresponding surface concentration, surface concentration change, surface refractive index, surface refractive index change, surface thickness and surface thickness change.

67. The method according to any one of Claims 51 to 66, characterised in that said determination of optical thickness images comprises:

- a) defining pixels, or clusters of pixels, on said first detector, each pixel or cluster of pixels corresponding to a respective one of a number of different zones on said surface,
- b) normalising and storing reflectance data obtained from the different zones without said thin layer structures so that the data are identical for all incident light angles/wavelengths,
- c) storing, during a suitable number of angular and/or wavelength scans over a predetermined period of time, in a memory the raw-data images detected by said pixel elements corresponding to said zones,
- d) storing, simultaneously, in a memory angular data and/or wavelength data detected by a pixel row or rows of said second detector corresponding to a constant reflectance zone on said surface, and time,
- e) calculating the monitored angle of incidence and/or wavelength as a function of time,
- f) storing in a memory a raw data image based on the calculated angle, time and/or wavelength,
- g) calculating a normalised image for each stored raw-data by use of the image-normalisation data in step b),
- h) storing the calculated angle, time and/or wavelength for the normalised image in a memory,



- i) assembling for each zone in said normalised image memory, the corresponding data for normalised reflectance/angle/wavelength/time into a reflectance curve versus angle, each angle corresponding to a specific time within the scan, and/or reflectance curve versus wavelength, each wavelength corresponding to a specific time within the scan,
- j) calculating for each zone in said memory, the angle and/or wavelength at the reflectance minimum, maximum and/or centroid for the reflectance curve, and a medium time for each scan,
- k) calculating for each zone in said memory, the angular shift, and/or wavelength shift versus a medium time for the scans,
- l) calculating for each zone, the change in surface concentration, refractive index or thickness from the angular shift, and/or wavelength shift, and
- m) presenting the simultaneous internal and/or relative changes in surface concentration, refractive index or thickness for selected zones as graphs or tables.

68. The method according to Claim 67, characterised in that said normalisation comprises:

- a) defining pixels, or clusters of pixels, on said first detector matrix, each pixel or cluster of pixels corresponding to a respective one of a number of different zones on said surface,
- b) defining from said zones/pixels or pixel clusters zones/pixel clusters to be used as reference zones,
- c) calibrating the angle and/or wavelength measurement by calculating the relation between the position of a detected focused intensity curve and the known angle of incidence and/or wavelength,
- d) storing, during a suitable number of angular and/or wavelength scans, in a memory the raw-data images detected by said pixel or pixel clusters corresponding to each zone,

- e) storing, during a predetermined number of angular and/or wavelength scans, as a function of time in a second computer memory the angular data and/or wavelength data detected by said pixel row or rows corresponding to the constant reflectance zone,
- f) calculating the monitored angle of incidence and/or wavelength as a function of time,
- g) storing in a memory the related calculated angle and/or wavelength, time, and raw data image,
- h) contacting said surface with a medium having a refractive index enabling a total internal reflectance at all said zones,
- i) calculating a reflectance normalisation data matrix for each raw-data image stored in said raw-data image memory, and
- j) storing in a memory the calculated angle, and/or wavelength, time, and image-normalisation data.

69. The method according to Claim 67 or 68, characterised in that the method comprises:

selecting said clusters of pixels on said detector matrix so that each cluster corresponds to the position of a respective zone on said surface, and that at least one pixel row corresponds to the position of a constant reflectance zone on said surface, and

assigning a specific centre-pixel to each of the imaged zones and a cluster of neighbour-pixels around this centre-pixel as a function of at least one of the size of the image of the sensor-zone, the geometry of the image of the zone, the size of the pixels of the detector matrix, the detected difference in reflectance for neighbour-pixels, the difference in electronic light-sensitivity and noise for different numbers of pixels and geometry of the pixel pattern within a cluster, and the integration time of the electronic average-response of the pixels.

70. The method according to Claim 69, characterised in that the assignment of the specific centre-pixels corresponding to each of the imaged surface zones and to the constant reflectance zone are performed manually, and that the method further comprises:

defining a zone pattern to thereby initiate the automatic generation of a matching default centre-pixel pattern, and a position-matching and locking of this generated default pixel pattern to the image of the respective zones, and

visualising the pixel pattern and the image of the surface zone on a screen during the scanning of at least one of the angle and wavelength of incidence.

71. The method according to Claim 69 or 70, characterised in that the assignment of the specific centre-pixel corresponding to each imaged surface zone, and of the specific pixel row or rows to the constant reflectance zone are performed automatically and that the method further comprises:


defining a surface zone pattern to thereby initiate the automatic generation of a matching default centre-pixel pattern,

performing an image analysis to determine the positions and borders of the surface zones within the image,

position-matching and locking the generated default pixel pattern to the determined image of the surface zones, and

visualising the pixel pattern and the image of the surface zone on a screen during the scanning of at least one of the angle and wavelength of incidence.

72. The method according to any one of Claims 51 to 66, characterised in that said light for monitoring angle and/or wavelength passes through at least one aperture in at least one obscuration.



- 56 -

73. An optical apparatus substantially as hereinbefore described with reference to the accompanying drawings.

74. A method of using an optical apparatus substantially as hereinbefore described with  
5 reference to the accompanying drawings.

DATED this 11th day of August, 2000

**Biacore AB**

10 By its Patent Attorneys

DAVIES COLLISON CAVE

5  
6  
7  
8  
9  
10  
11  
12  
13  
14  
15  
16  
17  
18  
19  
20  
21  
22  
23  
24  
25  
26  
27  
28  
29  
30  
31  
32  
33  
34  
35  
36  
37  
38  
39  
40  
41  
42  
43  
44  
45  
46  
47  
48  
49  
50  
51  
52  
53  
54  
55  
56  
57  
58  
59  
60  
61  
62  
63  
64  
65  
66  
67  
68  
69  
70  
71  
72  
73  
74  
75  
76  
77  
78  
79  
80  
81  
82  
83  
84  
85  
86  
87  
88  
89  
90  
91  
92  
93  
94  
95  
96  
97  
98  
99  
100  
101  
102  
103  
104  
105  
106  
107  
108  
109  
110  
111  
112  
113  
114  
115  
116  
117  
118  
119  
120  
121  
122  
123  
124  
125  
126  
127  
128  
129  
130  
131  
132  
133  
134  
135  
136  
137  
138  
139  
140  
141  
142  
143  
144  
145  
146  
147  
148  
149  
150  
151  
152  
153  
154  
155  
156  
157  
158  
159  
160  
161  
162  
163  
164  
165  
166  
167  
168  
169  
170  
171  
172  
173  
174  
175  
176  
177  
178  
179  
180  
181  
182  
183  
184  
185  
186  
187  
188  
189  
190  
191  
192  
193  
194  
195  
196  
197  
198  
199  
200  
201  
202  
203  
204  
205  
206  
207  
208  
209  
210  
211  
212  
213  
214  
215  
216  
217  
218  
219  
220  
221  
222  
223  
224  
225  
226  
227  
228  
229  
230  
231  
232  
233  
234  
235  
236  
237  
238  
239  
240  
241  
242  
243  
244  
245  
246  
247  
248  
249  
250  
251  
252  
253  
254  
255  
256  
257  
258  
259  
260  
261  
262  
263  
264  
265  
266  
267  
268  
269  
270  
271  
272  
273  
274  
275  
276  
277  
278  
279  
280  
281  
282  
283  
284  
285  
286  
287  
288  
289  
290  
291  
292  
293  
294  
295  
296  
297  
298  
299  
300  
301  
302  
303  
304  
305  
306  
307  
308  
309  
310  
311  
312  
313  
314  
315  
316  
317  
318  
319  
320  
321  
322  
323  
324  
325  
326  
327  
328  
329  
330  
331  
332  
333  
334  
335  
336  
337  
338  
339  
340  
341  
342  
343  
344  
345  
346  
347  
348  
349  
350  
351  
352  
353  
354  
355  
356  
357  
358  
359  
360  
361  
362  
363  
364  
365  
366  
367  
368  
369  
370  
371  
372  
373  
374  
375  
376  
377  
378  
379  
380  
381  
382  
383  
384  
385  
386  
387  
388  
389  
390  
391  
392  
393  
394  
395  
396  
397  
398  
399  
400  
401  
402  
403  
404  
405  
406  
407  
408  
409  
410  
411  
412  
413  
414  
415  
416  
417  
418  
419  
420  
421  
422  
423  
424  
425  
426  
427  
428  
429  
430  
431  
432  
433  
434  
435  
436  
437  
438  
439  
440  
441  
442  
443  
444  
445  
446  
447  
448  
449  
450  
451  
452  
453  
454  
455  
456  
457  
458  
459  
460  
461  
462  
463  
464  
465  
466  
467  
468  
469  
470  
471  
472  
473  
474  
475  
476  
477  
478  
479  
480  
481  
482  
483  
484  
485  
486  
487  
488  
489  
490  
491  
492  
493  
494  
495  
496  
497  
498  
499  
500  
501  
502  
503  
504  
505  
506  
507  
508  
509  
510  
511  
512  
513  
514  
515  
516  
517  
518  
519  
520  
521  
522  
523  
524  
525  
526  
527  
528  
529  
530  
531  
532  
533  
534  
535  
536  
537  
538  
539  
540  
541  
542  
543  
544  
545  
546  
547  
548  
549  
550  
551  
552  
553  
554  
555  
556  
557  
558  
559  
560  
561  
562  
563  
564  
565  
566  
567  
568  
569  
570  
571  
572  
573  
574  
575  
576  
577  
578  
579  
580  
581  
582  
583  
584  
585  
586  
587  
588  
589  
590  
591  
592  
593  
594  
595  
596  
597  
598  
599  
600  
601  
602  
603  
604  
605  
606  
607  
608  
609  
610  
611  
612  
613  
614  
615  
616  
617  
618  
619  
620  
621  
622  
623  
624  
625  
626  
627  
628  
629  
630  
631  
632  
633  
634  
635  
636  
637  
638  
639  
640  
641  
642  
643  
644  
645  
646  
647  
648  
649  
650  
651  
652  
653  
654  
655  
656  
657  
658  
659  
660  
661  
662  
663  
664  
665  
666  
667  
668  
669  
670  
671  
672  
673  
674  
675  
676  
677  
678  
679  
680  
681  
682  
683  
684  
685  
686  
687  
688  
689  
690  
691  
692  
693  
694  
695  
696  
697  
698  
699  
700  
701  
702  
703  
704  
705  
706  
707  
708  
709  
710  
711  
712  
713  
714  
715  
716  
717  
718  
719  
720  
721  
722  
723  
724  
725  
726  
727  
728  
729  
730  
731  
732  
733  
734  
735  
736  
737  
738  
739  
740  
741  
742  
743  
744  
745  
746  
747  
748  
749  
750  
751  
752  
753  
754  
755  
756  
757  
758  
759  
760  
761  
762  
763  
764  
765  
766  
767  
768  
769  
770  
771  
772  
773  
774  
775  
776  
777  
778  
779  
780  
781  
782  
783  
784  
785  
786  
787  
788  
789  
790  
791  
792  
793  
794  
795  
796  
797  
798  
799  
800  
801  
802  
803  
804  
805  
806  
807  
808  
809  
810  
811  
812  
813  
814  
815  
816  
817  
818  
819  
820  
821  
822  
823  
824  
825  
826  
827  
828  
829  
830  
831  
832  
833  
834  
835  
836  
837  
838  
839  
840  
841  
842  
843  
844  
845  
846  
847  
848  
849  
850  
851  
852  
853  
854  
855  
856  
857  
858  
859  
860  
861  
862  
863  
864  
865  
866  
867  
868  
869  
870  
871  
872  
873  
874  
875  
876  
877  
878  
879  
880  
881  
882  
883  
884  
885  
886  
887  
888  
889  
890  
891  
892  
893  
894  
895  
896  
897  
898  
899  
900  
901  
902  
903  
904  
905  
906  
907  
908  
909  
910  
911  
912  
913  
914  
915  
916  
917  
918  
919  
920  
921  
922  
923  
924  
925  
926  
927  
928  
929  
930  
931  
932  
933  
934  
935  
936  
937  
938  
939  
940  
941  
942  
943  
944  
945  
946  
947  
948  
949  
950  
951  
952  
953  
954  
955  
956  
957  
958  
959  
960  
961  
962  
963  
964  
965  
966  
967  
968  
969  
970  
971  
972  
973  
974  
975  
976  
977  
978  
979  
980  
981  
982  
983  
984  
985  
986  
987  
988  
989  
990  
991  
992  
993  
994  
995  
996  
997  
998  
999  
1000  
1001  
1002  
1003  
1004  
1005  
1006  
1007  
1008  
1009  
1010  
1011  
1012  
1013  
1014  
1015  
1016  
1017  
1018  
1019  
1020  
1021  
1022  
1023  
1024  
1025  
1026  
1027  
1028  
1029  
1030  
1031  
1032  
1033  
1034  
1035  
1036  
1037  
1038  
1039  
1040  
1041  
1042  
1043  
1044  
1045  
1046  
1047  
1048  
1049  
1050  
1051  
1052  
1053  
1054  
1055  
1056  
1057  
1058  
1059  
1060  
1061  
1062  
1063  
1064  
1065  
1066  
1067  
1068  
1069  
1070  
1071  
1072  
1073  
1074  
1075  
1076  
1077  
1078  
1079  
1080  
1081  
1082  
1083  
1084  
1085  
1086  
1087  
1088  
1089  
1090  
1091  
1092  
1093  
1094  
1095  
1096  
1097  
1098  
1099  
1100  
1101  
1102  
1103  
1104  
1105  
1106  
1107  
1108  
1109  
1110  
1111  
1112  
1113  
1114  
1115  
1116  
1117  
1118  
1119  
1120  
1121  
1122  
1123  
1124  
1125  
1126  
1127  
1128  
1129  
1130  
1131  
1132  
1133  
1134  
1135  
1136  
1137  
1138  
1139  
1140  
1141  
1142  
1143  
1144  
1145  
1146  
1147  
1148  
1149  
1150  
1151  
1152  
1153  
1154  
1155  
1156  
1157  
1158  
1159  
1160  
1161  
1162  
1163  
1164  
1165  
1166  
1167  
1168  
1169  
1170  
1171  
1172  
1173  
1174  
1175  
1176  
1177  
1178  
1179  
1180  
1181  
1182  
1183  
1184  
1185  
1186  
1187  
1188  
1189  
1190  
1191  
1192  
1193  
1194  
1195  
1196  
1197  
1198  
1199  
1200  
1201  
1202  
1203  
1204  
1205  
1206  
1207  
1208  
1209  
1210  
1211  
1212  
1213  
1214  
1215  
1216  
1217  
1218  
1219  
1220  
1221  
1222  
1223  
1224  
1225  
1226  
1227  
1228  
1229  
1230  
1231  
1232  
1233  
1234  
1235  
1236  
1237  
1238  
1239  
1240  
1241  
1242  
1243  
1244  
1245  
1246  
1247  
1248  
1249  
1250  
1251  
1252  
1253  
1254  
1255  
1256  
1257  
1258  
1259  
1260  
1261  
1262  
1263  
1264  
1265  
1266  
1267  
1268  
1269  
1270  
1271  
1272  
1273  
1274  
1275  
1276  
1277  
1278  
1279  
1280  
1281  
1282  
1283  
1284  
1285  
1286  
1287  
1288  
1289  
1290  
1291  
1292  
1293  
1294  
1295  
1296  
1297  
1298  
1299  
1300  
1301  
1302  
1303  
1304  
1305  
1306  
1307  
1308  
1309  
1310  
1311  
1312  
1313  
1314  
1315  
1316  
1317  
1318  
1319  
1320  
1321  
1322  
1323  
1324  
1325  
1326  
1327  
1328  
1329  
1330  
1331  
1332  
1333  
1334  
1335  
1336  
1337  
1338  
1339  
1340  
1341  
1342  
1343  
1344  
1345  
1346  
1347  
1348  
1349  
1350  
1351  
1352  
1353  
1354  
1355  
1356  
1357  
1358  
1359  
1360  
1361  
1362  
1363  
1364  
1365  
1366  
1367  
1368  
1369  
1370  
1371  
1372  
1373  
1374  
1375  
1376  
1377  
1378  
1379  
1380  
1381  
1382  
1383  
1384  
1385  
1386  
1387  
1388  
1389  
1390  
1391  
1392  
1393  
1394  
1395  
1396  
1397  
1398  
1399  
1400  
1401  
1402  
1403  
1404  
1405  
1406  
1407  
1408  
1409  
1410  
1411  
1412  
1413  
1414  
1415  
1416  
1417  
1418  
1419  
1420  
1421  
1422  
1423  
1424  
1425  
1426  
1427  
1428  
1429  
1430  
1431  
1432  
1433  
1434  
1435  
1436  
1437  
1438  
1439  
1440  
1441  
1442  
1443  
1444  
1445  
1446  
1447  
1448  
1449  
1450  
1451  
1452  
1453  
1454  
1455  
1456  
1457  
1458  
1459  
1460  
1461  
1462  
1463  
1464  
1465  
1466  
1467  
1468  
1469  
1470  
1471  
1472  
1473  
1474  
1475  
1476  
1477  
1478  
1479  
1480  
1481  
1482  
1483  
1484  
1485  
1486  
1487  
1488  
1489  
1490  
1491  
1492  
1493  
1494  
1495  
1496  
1497  
1498  
1499  
1500  
1501  
1502  
1503  
1504  
1505  
1506  
1507  
1508  
1509  
1510  
1511  
1512  
1513  
1514  
1515  
1516  
1517  
1518  
1519  
1520  
1521  
1522  
1523  
1524  
1525  
1526  
1527  
1528  
1529  
1530  
1531  
1532  
1533  
1534  
1535  
1536  
1537  
1538  
1539  
1540  
1541  
1542  
1543  
1544  
1545  
1546  
1547  
1548  
1549  
1550  
1551  
1552  
1553  
1554  
1555  
1556  
1557  
1558  
1559  
1560  
1561  
1562  
1563  
1564  
1565  
1566  
1567  
1568  
1569  
1570  
1571  
1572  
1573  
1574  
1575  
1576  
1577  
1578  
1579  
1580  
1581  
1582  
1583  
1584  
1585  
1586  
1587  
1588  
1589  
1590  
1591  
1592  
1593  
1594  
1595  
1596  
1597  
1598  
1599  
1600  
1601  
1602  
1603  
1604  
1605  
1606  
1607  
1608  
1609  
1610  
1611  
1612  
1613  
1614  
1615  
1616  
1617  
1618  
1619  
1620  
1621  
1622  
1623  
1624  
1625  
1626  
1627  
1628  
1629  
1630  
1631  
1632  
1633  
1634  
1635  
1636  
1637  
1638  
1639  
1640  
1641  
1642  
1643  
1644  
1645  
1646  
1647  
1648  
1649  
1650  
1651  
1652  
1653  
1654  
1655  
1656  
1657  
1658  
1659  
1660  
1661  
1662  
1663  
1664  
1665  
1666  
1667  
1668  
1669  
1670  
1671  
1672  
1673  
1674  
1675  
1676  
1677  
1678  
1679  
1680  
1681  
1682  
1683  
1684  
1685  
1686  
1687  
1688  
1689  
1690  
1691  
1692  
1693  
1694  
1695  
1696  
1697  
1698  
1699  
1700  
1701  
1702  
1703  
1704  
1705  
1706  
1707  
1708  
1709  
1710  
1711  
1712  
1713  
1714  
1715  
1716  
1717  
1718  
1719  
1720  
1721  
1722  
1723  
1724  
1725  
1726  
1727  
1728  
1729  
1730  
1731  
1732  
1733  
1734  
1735  
1736  
1737  
1738  
1739  
1740  
1741  
1742  
1743  
1744  
1745  
1746  
1747  
1748  
1749  
1750  
1751  
1752  
1753  
1754  
1755  
1756  
1757  
1758  
1759  
1760  
1761  
1762  
1763  
1764  
1765  
1766  
1767  
1768  
1769  
1770  
1771  
1772  
1773  
1774  
1775  
1776  
1777  
1778  
1779  
1780  
1781  
1782  
1783  
1784  
1785  
1786  
1787  
1788  
1789  
1790  
1791  
1792  
1793  
1794  
1795  
1796  
1797  
1798  
1799  
1800  
1801  
1802  
1803  
1804  
1805  
1806  
1807  
1808  
1809  
1810  
1811  
1812  
1813  
1814  
1815  
1816  
1817  
1818  
1819  
1820  
1821  
1822  
1823  
1824  
1825  
1826  
1827  
1828  
1829  
1830  
1831  
1832  
1833  
1834  
1835  
1836  
1837  
1838  
1839  
1840  
1841  
1842  
1843  
1844  
1845  
1846  
1847  
1848  
1849  
1850  
1851  
1852  
1853  
1854  
1855  
1856  
1857  
1858  
1859  
1860  
1861  
1862  
1863  
1864  
1865  
1866  
1867  
1868  
1869  
1870  
1871  
1872  
1873  
1874  
1875  
1876  
1877  
1878  
1879  
1880  
1881  
1882  
1883  
1884  
1885  
1886  
1887  
1888  
1889  
1890  
1891  
1892  
1893  
1894  
1895  
1896  
1897  
1898  
1899  
1900  
1901  
1902  
1903  
1904  
1905  
1906  
1907  
1908  
1909  
1910  
1911  
1912  
1913  
1914  
1915  
1916  
1917  
1918  
1919  
1920  
1921  
1922  
1923  
1924  
1925  
1926  
1927  
1928  
1929  
1930  
1931  
1932  
1933  
1934  
1935  
1936  
1937  
1938  
1939  
1940  
1941  
1942  
1943  
1944  
1945  
1946  
1947  
1948  
1949  
1950  
1951  
1952  
1953  
1954  
1955  
1956  
1957  
1958  
1959  
1960  
1961  
1962  
1963  
1964  
1965  
1966  
1967  
1968  
1969  
1970  
1971  
1972  
1973  
1974  
1975  
1976  
1977  
1978  
1979  
1980  
1981  
1982  
1983  
1984  
1985  
1986  
1987  
1988  
1989  
1990  
1991  
1992  
1993  
1994  
1995  
1996  
1997  
1998  
1999  
2000  
2001  
2002  
2003  
2004  
2005  
2006  
2007  
2008  
2009  
2010  
2011  
2012  
2013  
2014  
2015  
2016  
2017  
2018  
2019  
2020  
2021  
2022  
2023  
2024  
2025  
2026  
2027  
2028  
2029  
2030  
2031  
2032  
2033  
2034  
2035  
2036  
2037  
2038  
2039  
2040  
2041  
2042  
2043  
2044  
2045  
2046  
2047  
2048  
2049  
2050  
2051  
2052  
2053  
2054  
2055  
2056  
2057  
2058  
2059  
2060  
2061  
2062  
2063  
2064  
2065  
2066  
2067  
2068  
2069  
2070  
2071  
2072  
2073  
2074  
2075  
2076  
2077  
2078  
2079  
2080  
2081  
2082  
2083  
2084  
2085  
2086  
2087  
2088  
2089  
2090  
2091  
2092  
2093  
2094  
2095  
2096  
2097  
2098  
2099  
2100  
2101  
2102  
2103  
2104  
2105  
2106  
2107  
2108  
2109  
2110  
2111  
2112  
2113  
2114  
2115  
2116  
2117  
2118  
2119  
2120  
2121  
2122  
2123  
2124  
2125  
2126  
2127  
2128  
2129  
2130  
2131  
2132  
2133  
2134  
2135  
2136  
2137  
2138  
2139  
2140  
2141  
2142  
2143  
2144  
2145  
2146  
2147  
2148  
2149  
2150  
2151  
2152  
2153  
2154  
2155  
2156  
2157  
2158  
2159  
2160  
2161  
2162  
2163  
2164  
2165  
2166  
2167  
2168  
2169  
2170  
2171  
2172  
2173  
2174  
2175  
2176  
2177  
2178  
2179  
2180  
2181  
2182  
2183  
2184

11 08 00 31:53

1/20

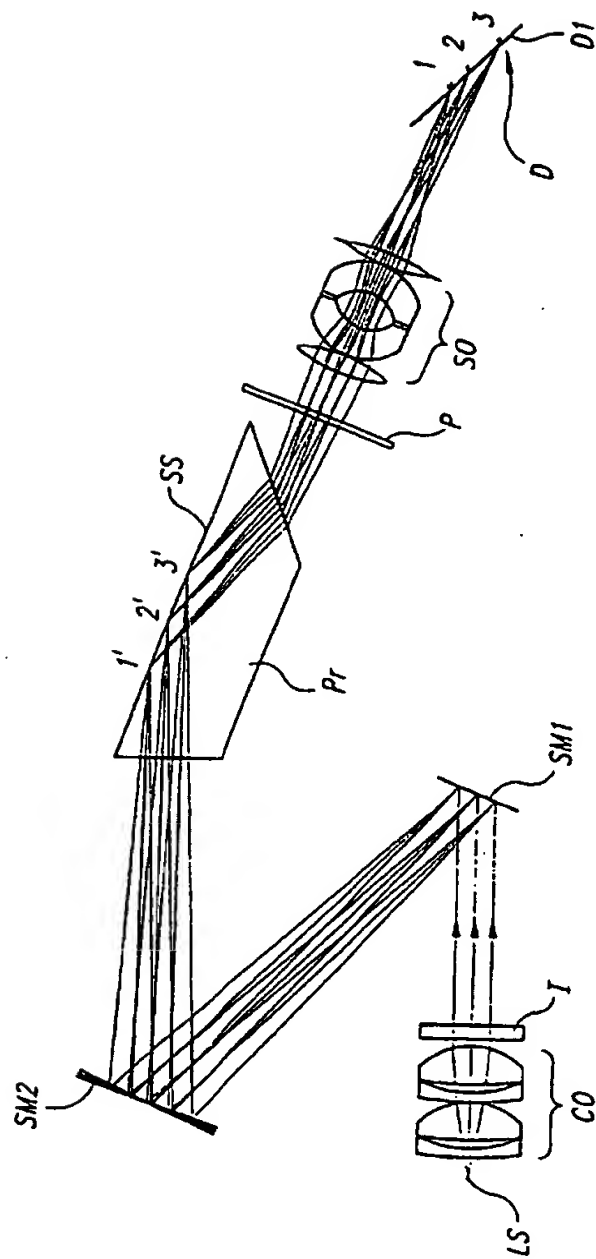


Fig. 1

11 00 00 51953

2/20

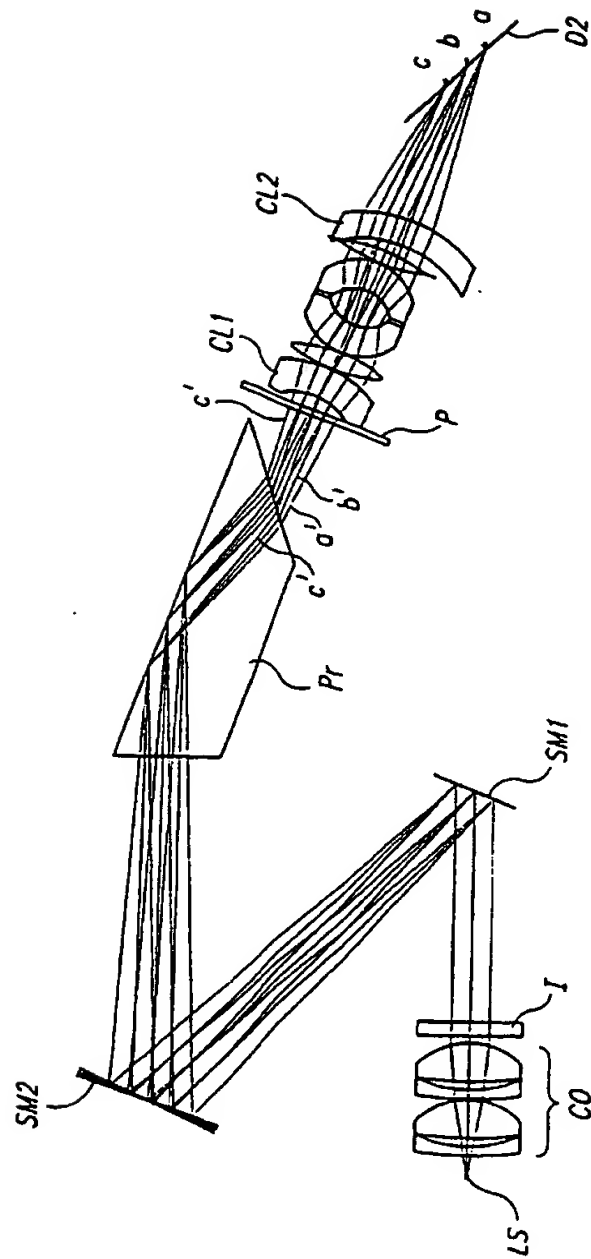


Fig. 2

11 08 00 31353

3/20

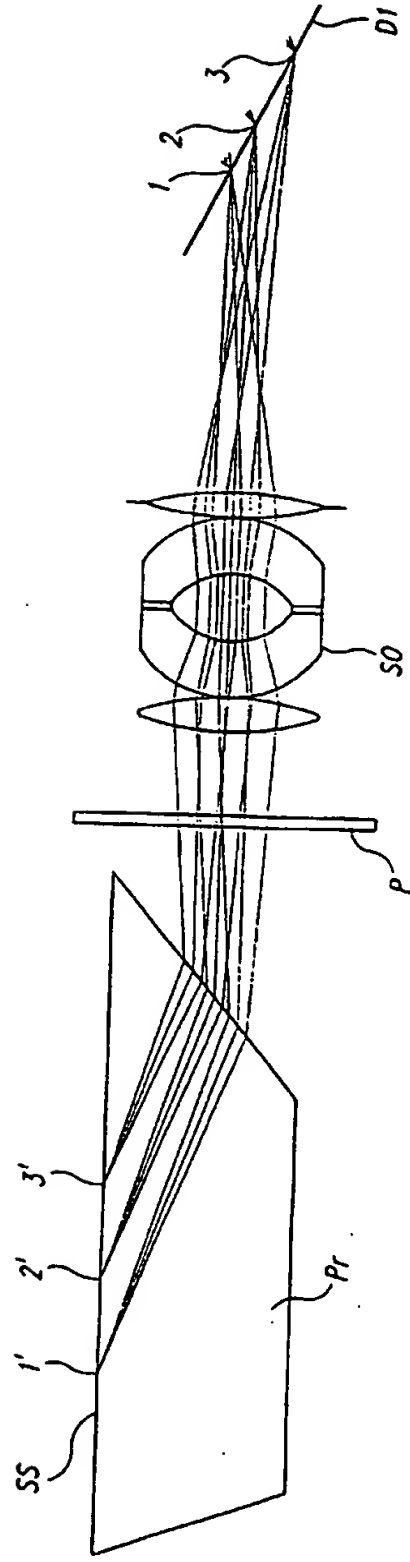


Fig. 3

11 00 00 3333

4/20

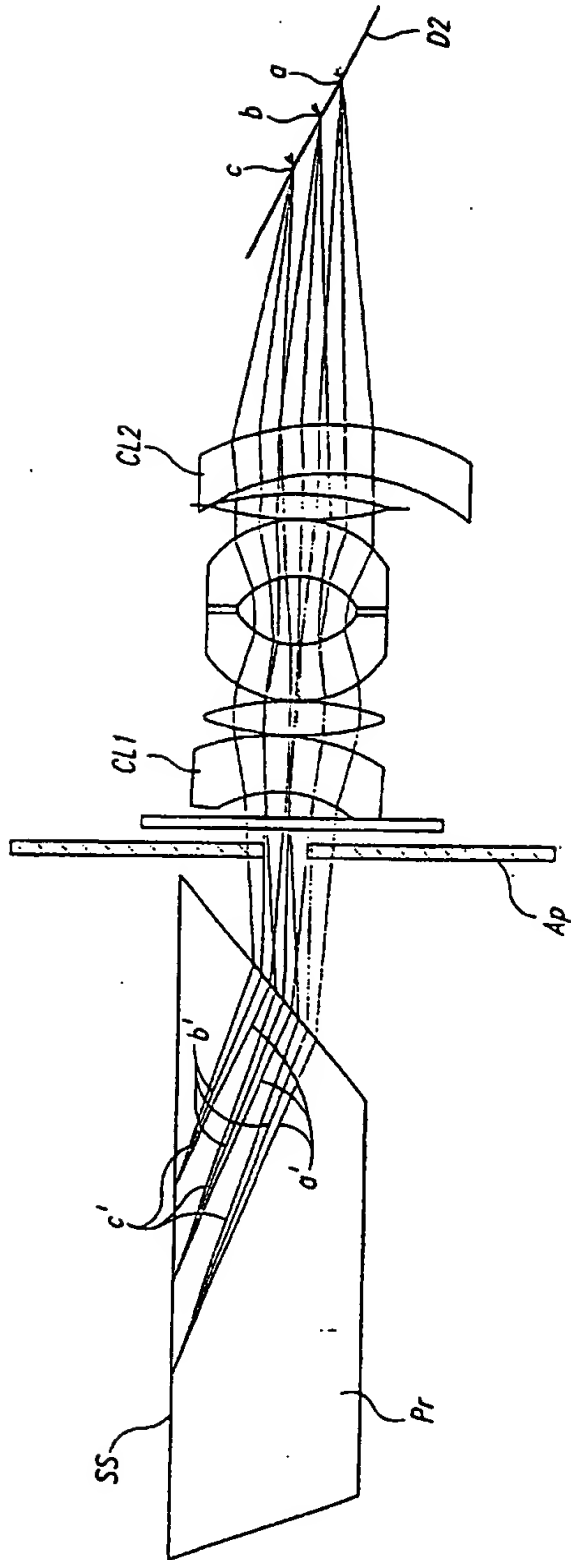


Fig. 4



11 08 00 31353

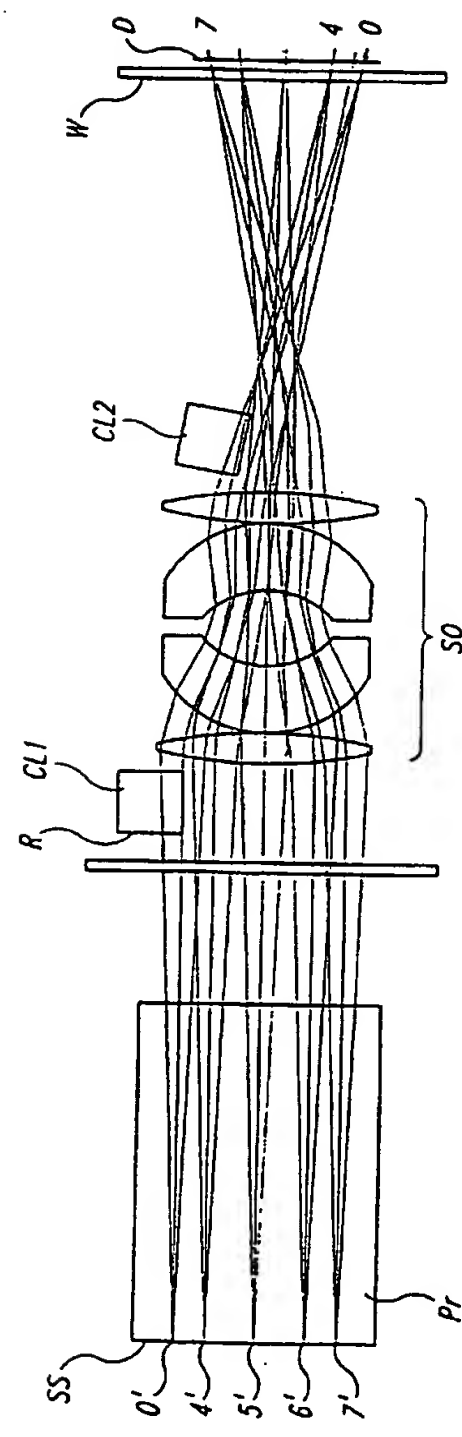


Fig. 5

11 88 00 51953

6/20

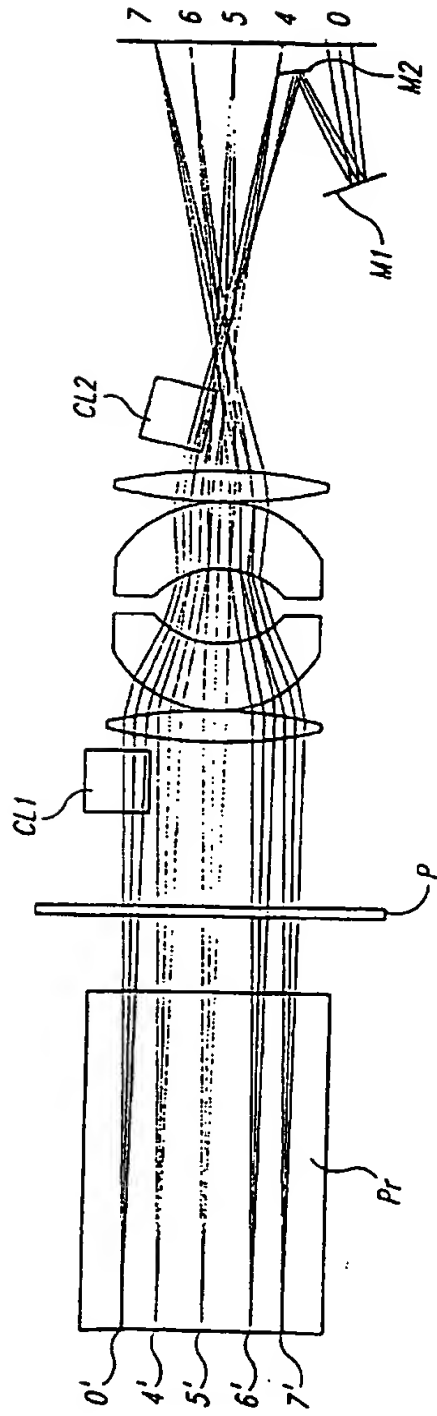


Fig. 6

11 00 00 5353

7/20

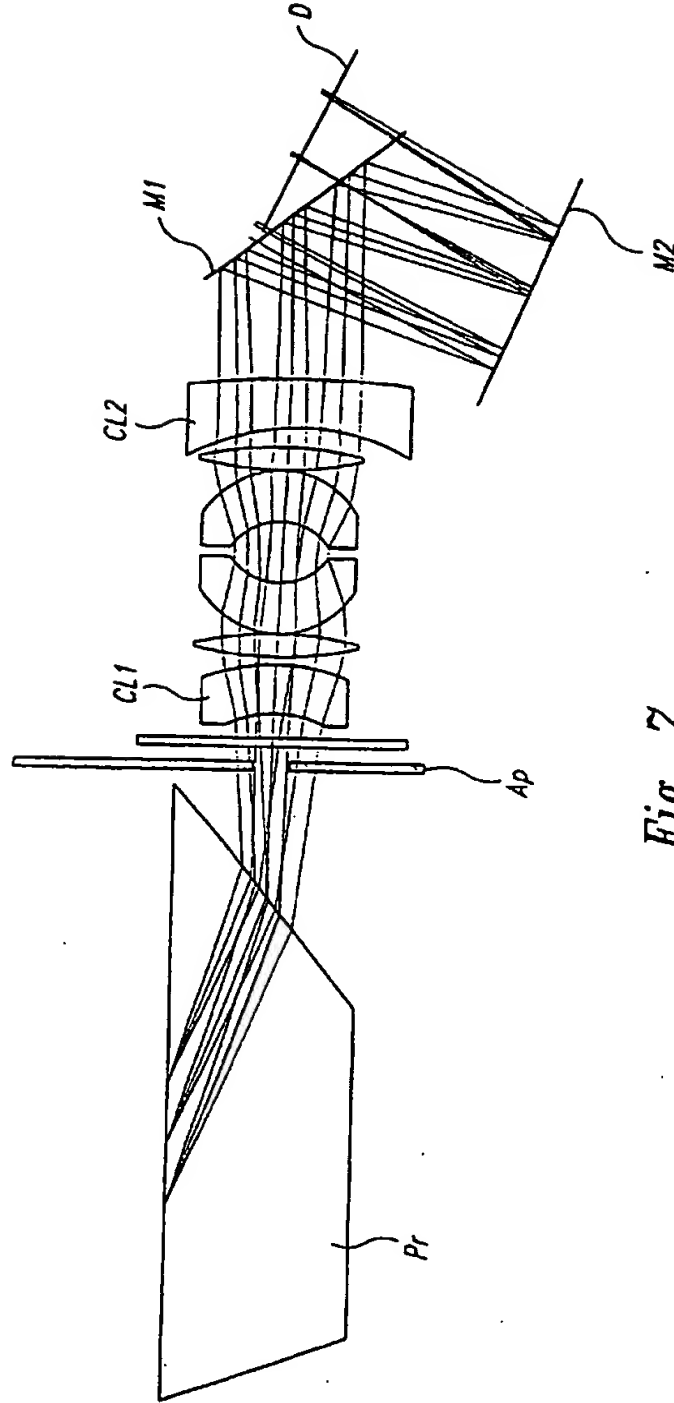


Fig. 7

8/20

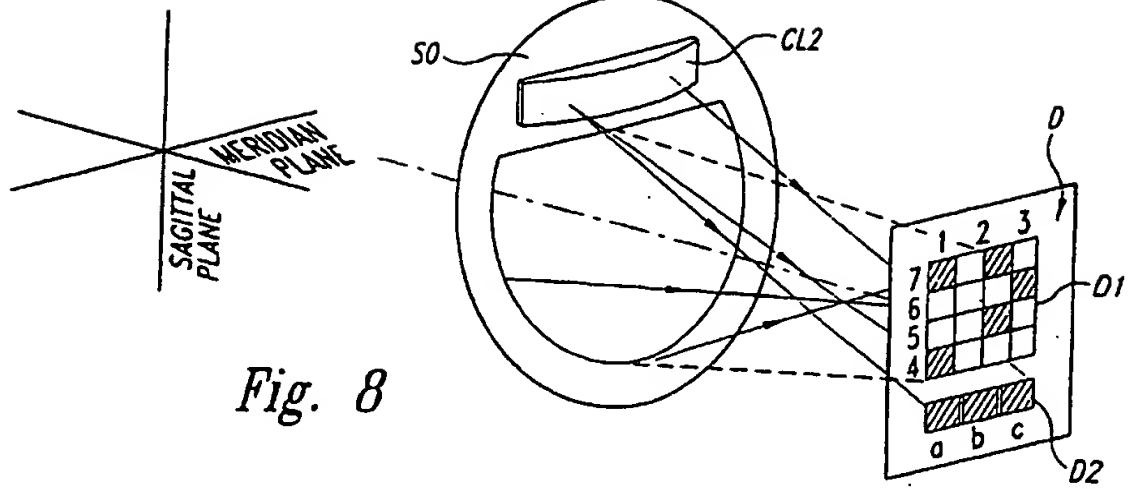


Fig. 8

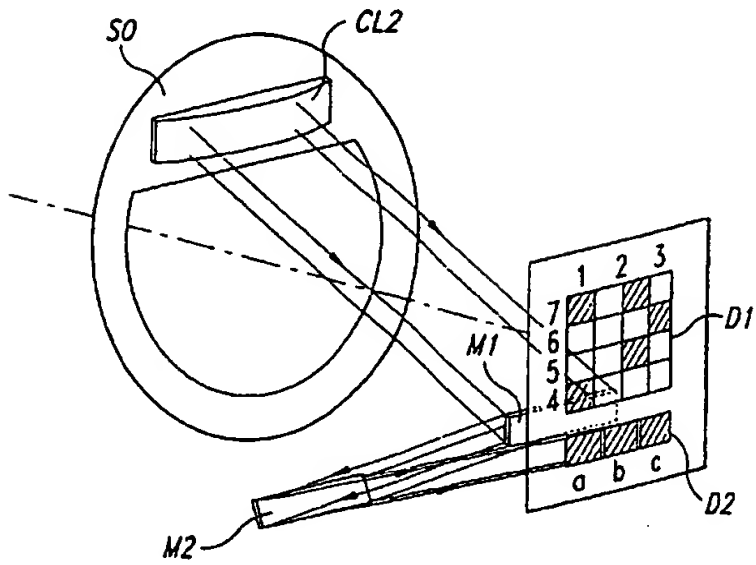


Fig. 9


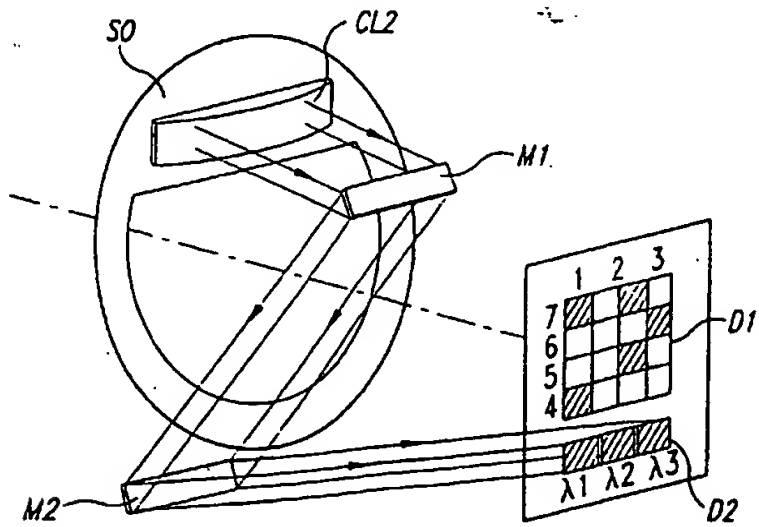


Fig. 10

11 00 00 31983

9/20

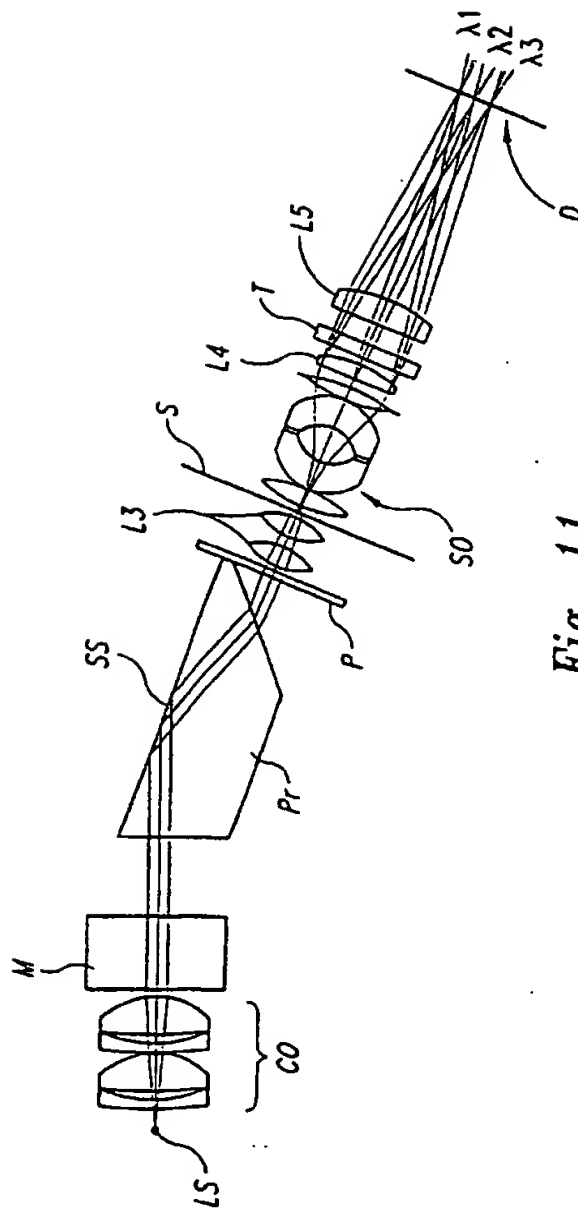

11 00 00 51053

10/20

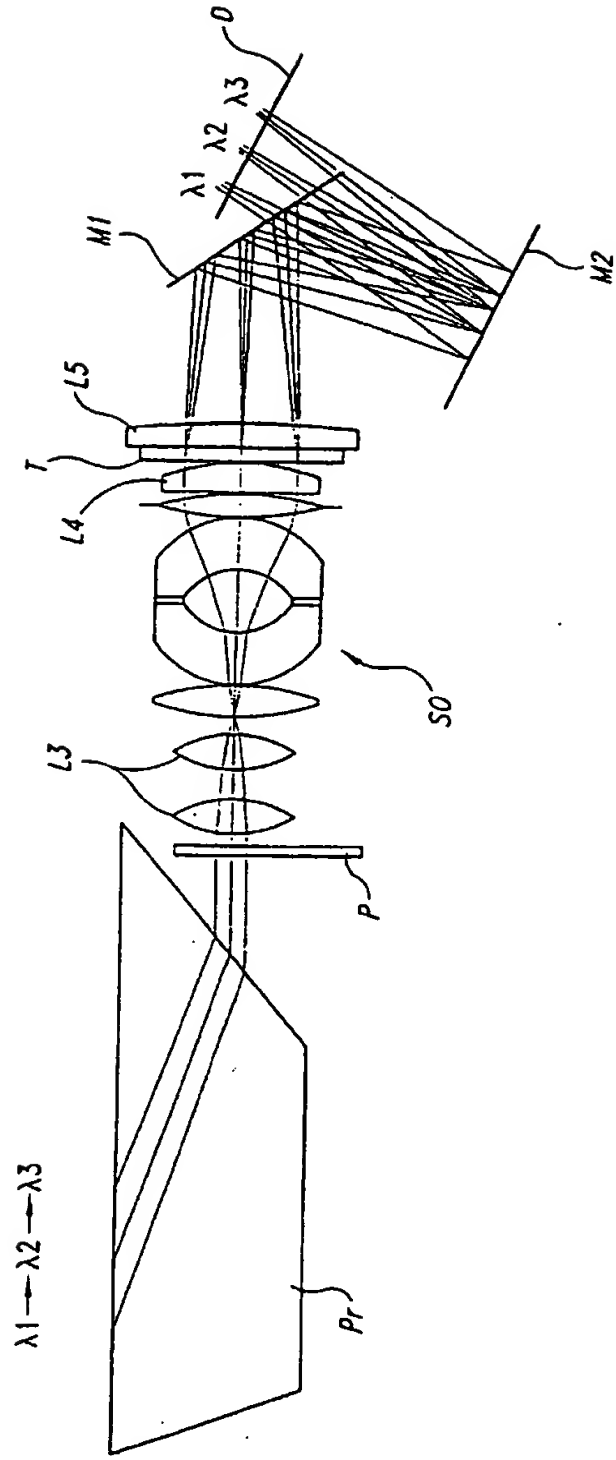


Fig. 12

11 08 00 53.953

11/20

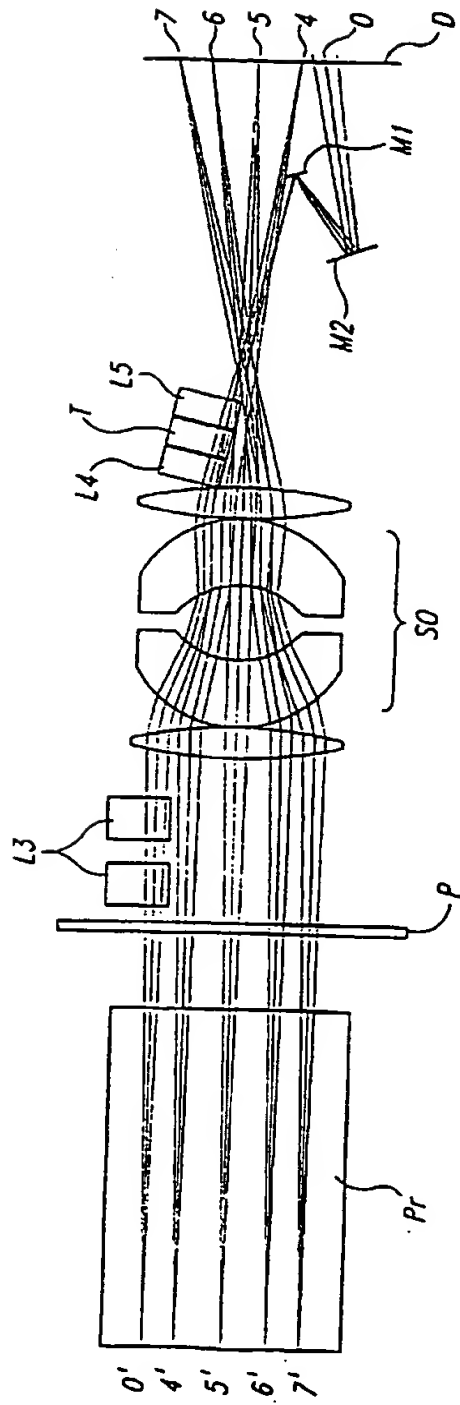


Fig. 13

11 08 08 5353

12/20

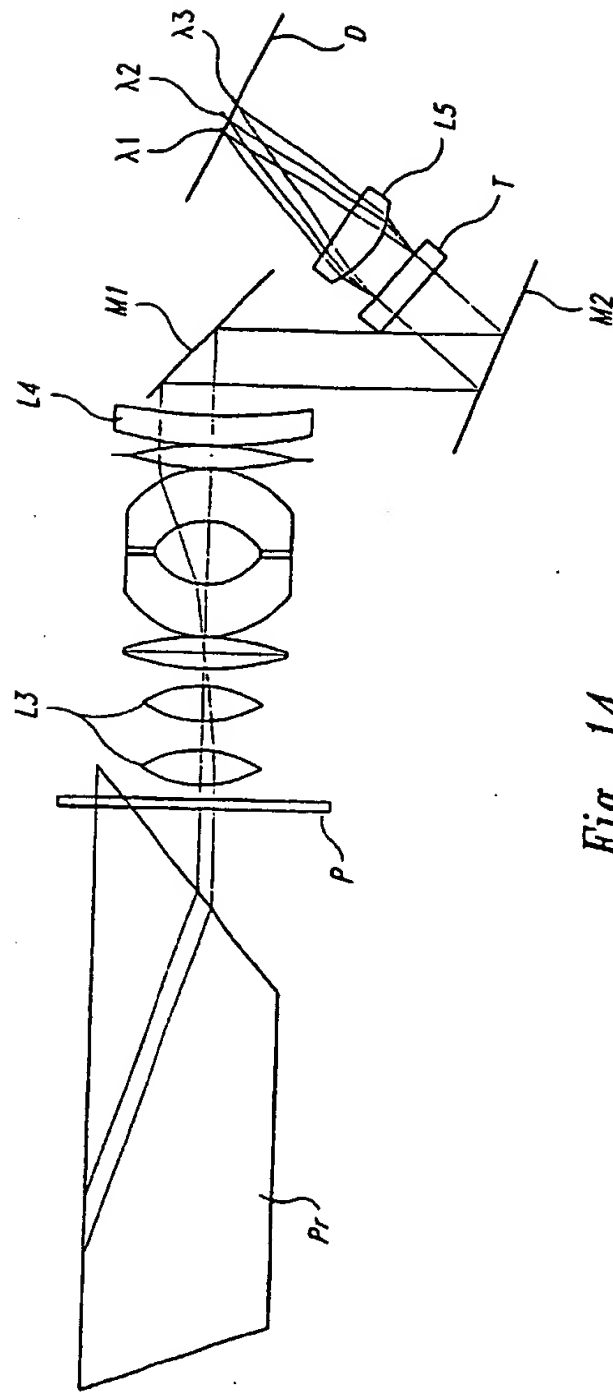


Fig. 14



11 08 00 3133

13/20

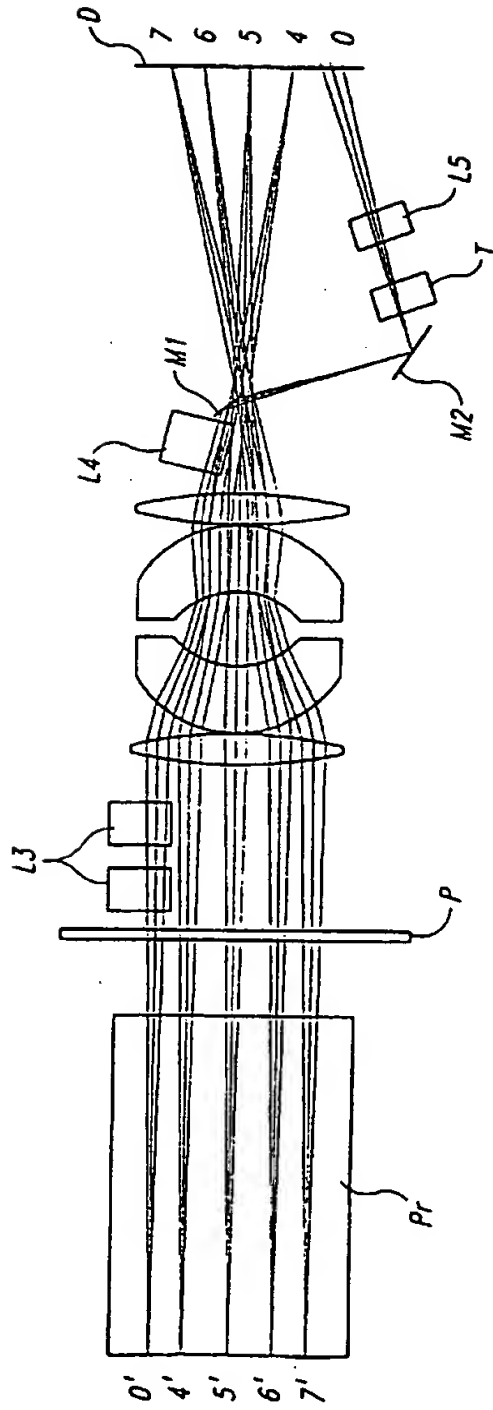


Fig. 15

11 08 00 31033

14/20

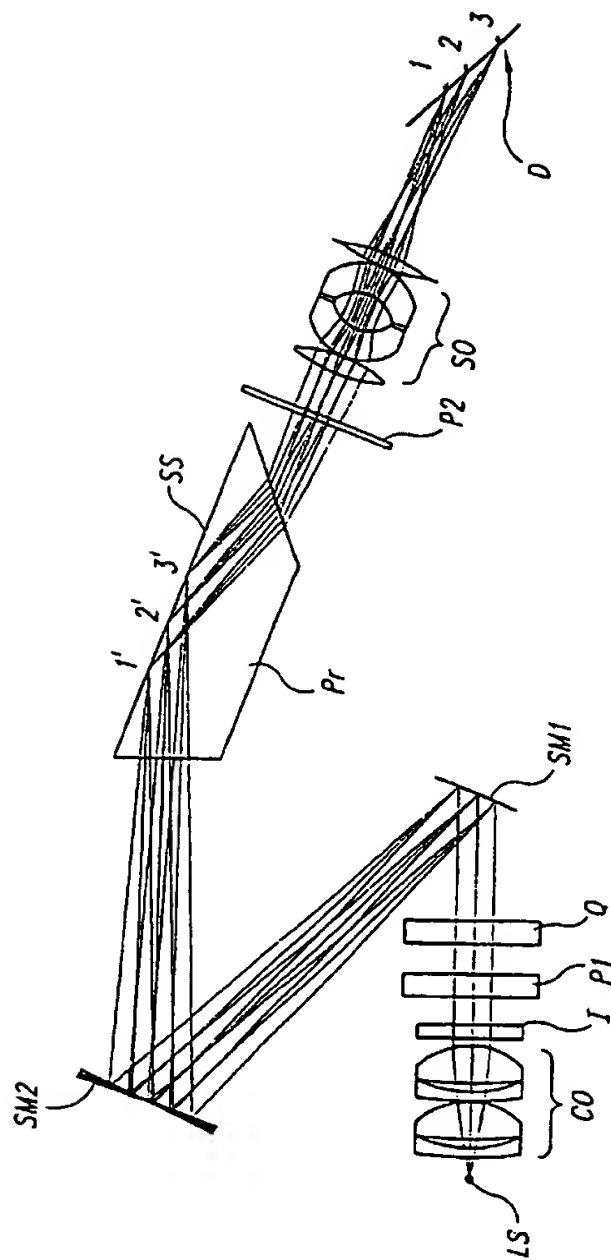


Fig. 16

11 08 08 51033

15/20

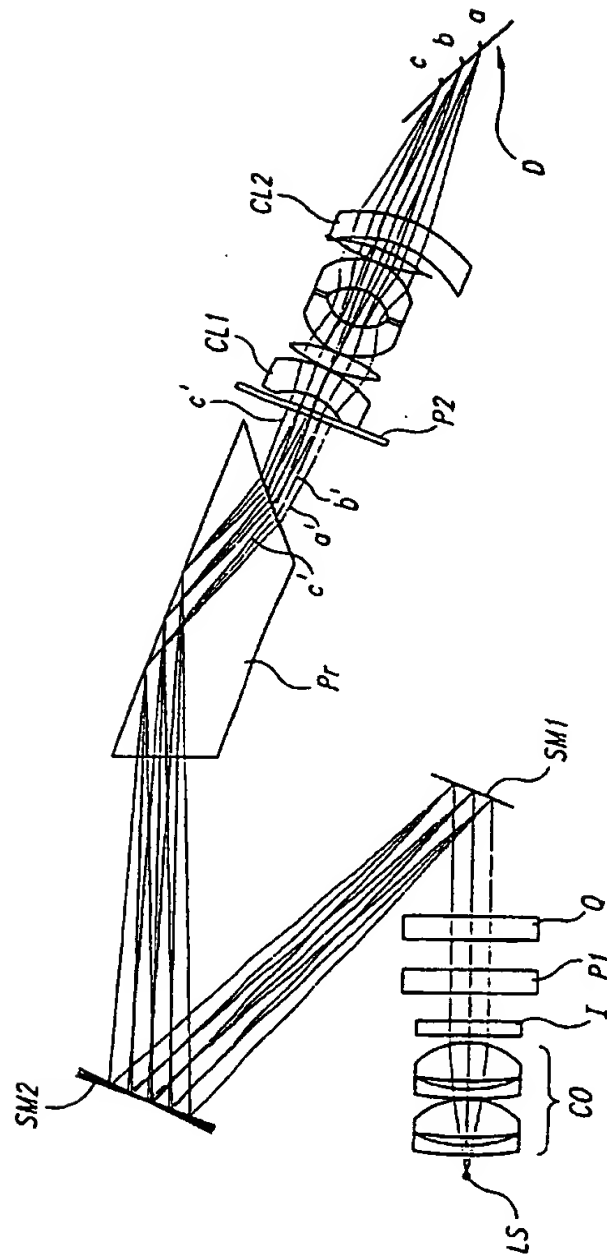


Fig. 17

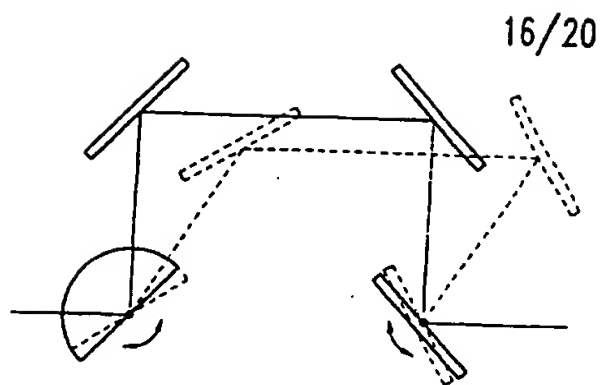


Fig. 18

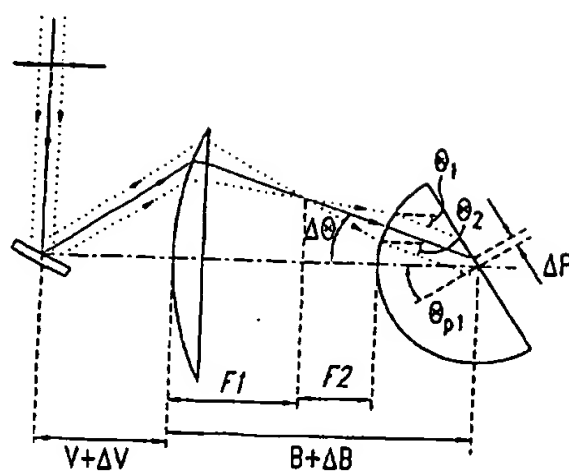


Fig. 19

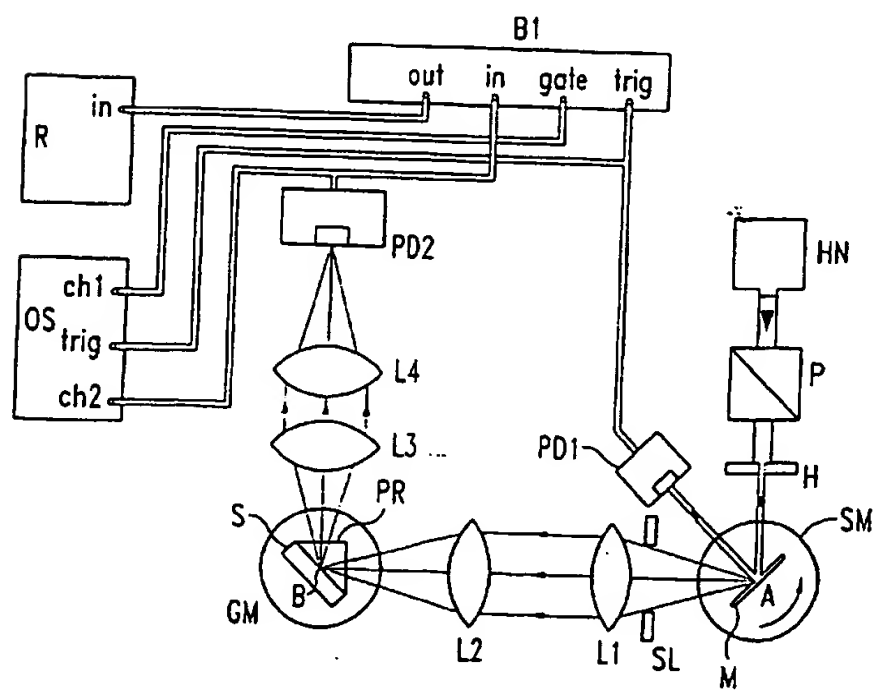
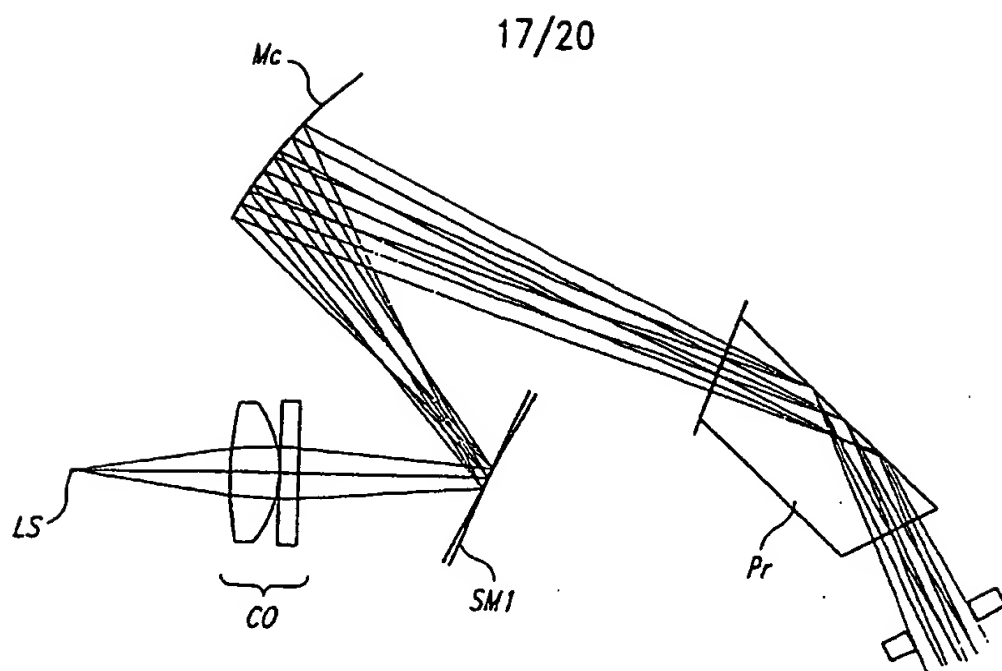
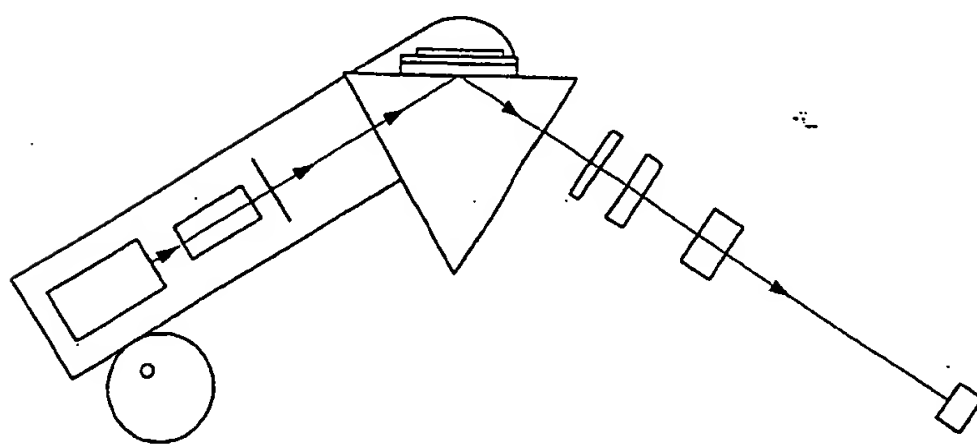


Fig. 20



*Fig. 21*



*Fig. 22*

11 08 00 5353

18/20

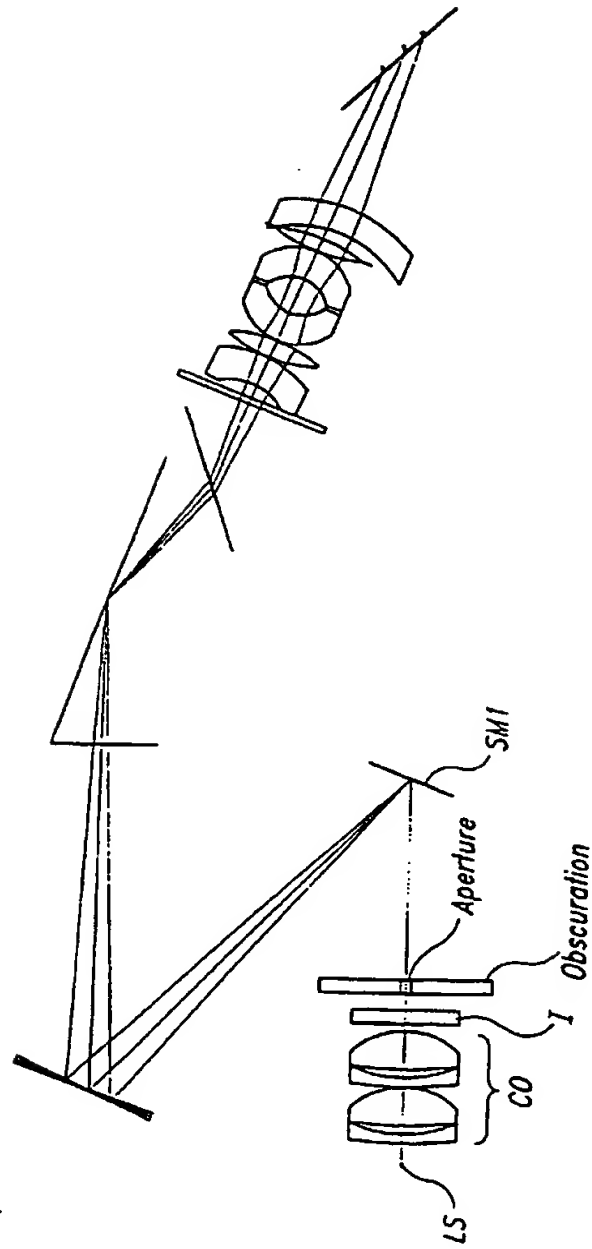
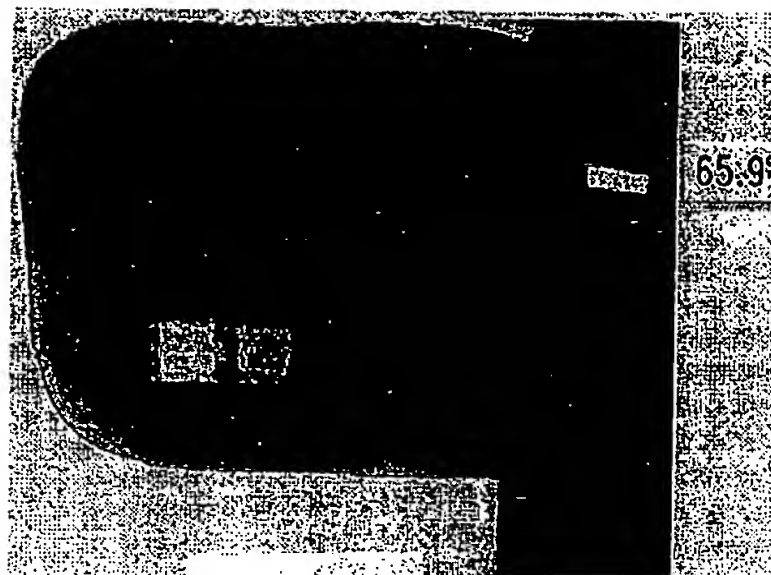
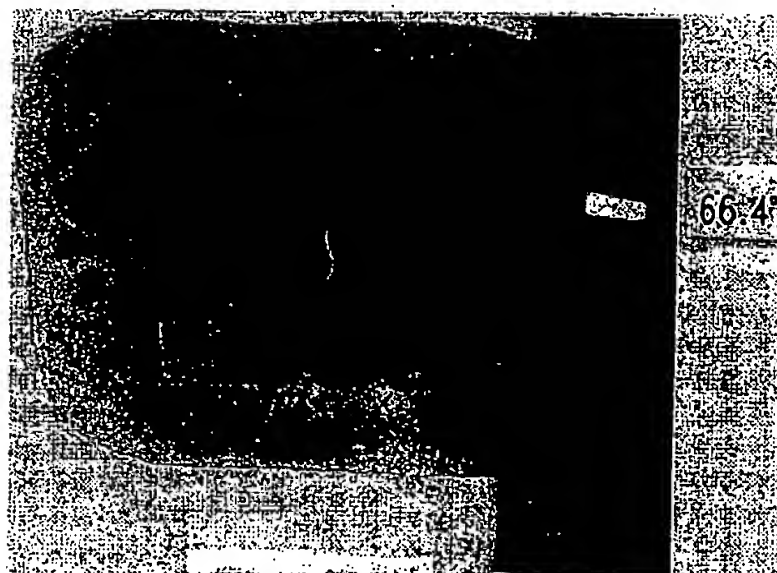


Fig. 23

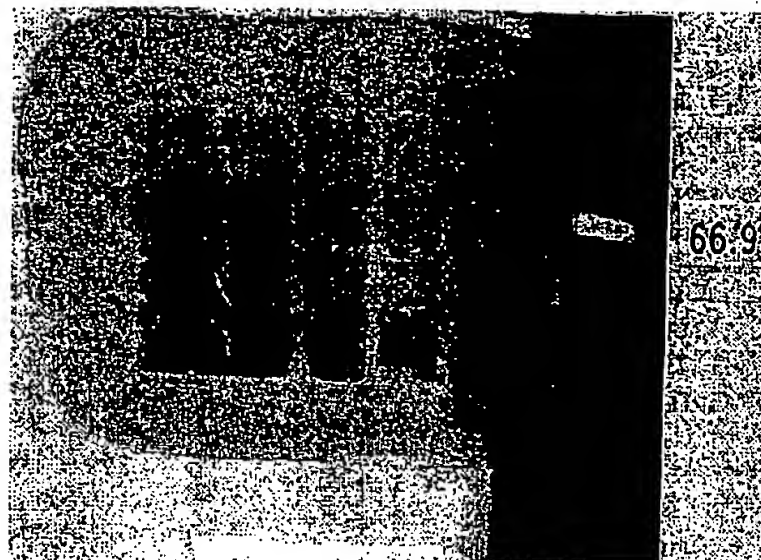


*Fig. 24A*

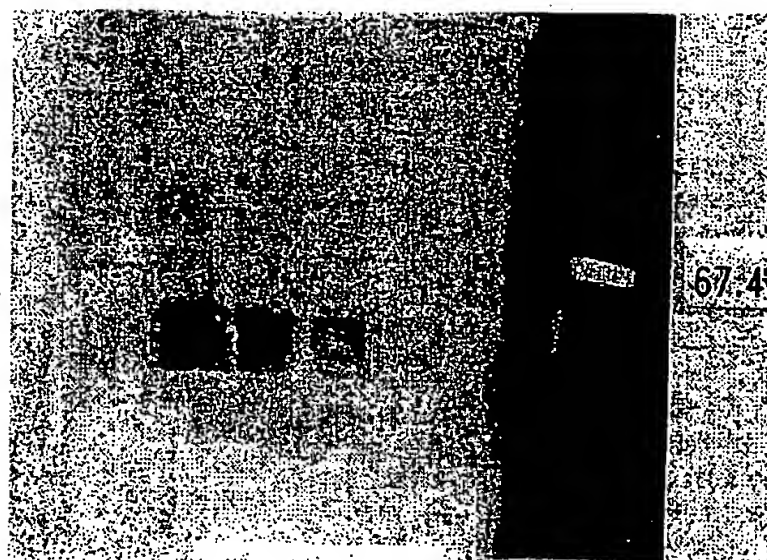


*Fig. 24B*

2  
3  
4  
5  
6  
7  
8  
9  
10  
11  
12  
13  
14  
15  
16  
17  
18  
19  
20



*Fig. 24C*



*Fig. 24D*

20/20



**This Page is Inserted by IFW Indexing and Scanning  
Operations and is not part of the Official Record**

## **BEST AVAILABLE IMAGES**

Defective images within this document are accurate representations of the original documents submitted by the applicant.

Defects in the images include but are not limited to the items checked:

- ☐ **BLACK BORDERS**
- ☐ **IMAGE CUT OFF AT TOP, BOTTOM OR SIDES**
- ☐ **FADED TEXT OR DRAWING**
- ☐ **BLURRED OR ILLEGIBLE TEXT OR DRAWING**
- ☐ **SKEWED/SLANTED IMAGES**
- ☐ **COLOR OR BLACK AND WHITE PHOTOGRAPHS**
- ☐ **GRAY SCALE DOCUMENTS**
- ☐ **LINES OR MARKS ON ORIGINAL DOCUMENT**
- ☐ **REFERENCE(S) OR EXHIBIT(S) SUBMITTED ARE POOR QUALITY.**
- ☐ **OTHER:** \_\_\_\_\_

**IMAGES ARE BEST AVAILABLE COPY.**

**As rescanning these documents will not correct the image problems checked, please do not report these problems to the IFW Image Problem Mailbox.**